

Sample Name : PTH(1-34),bovine
 Cat. No. : RP10364
 Lot. No. : CD19907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

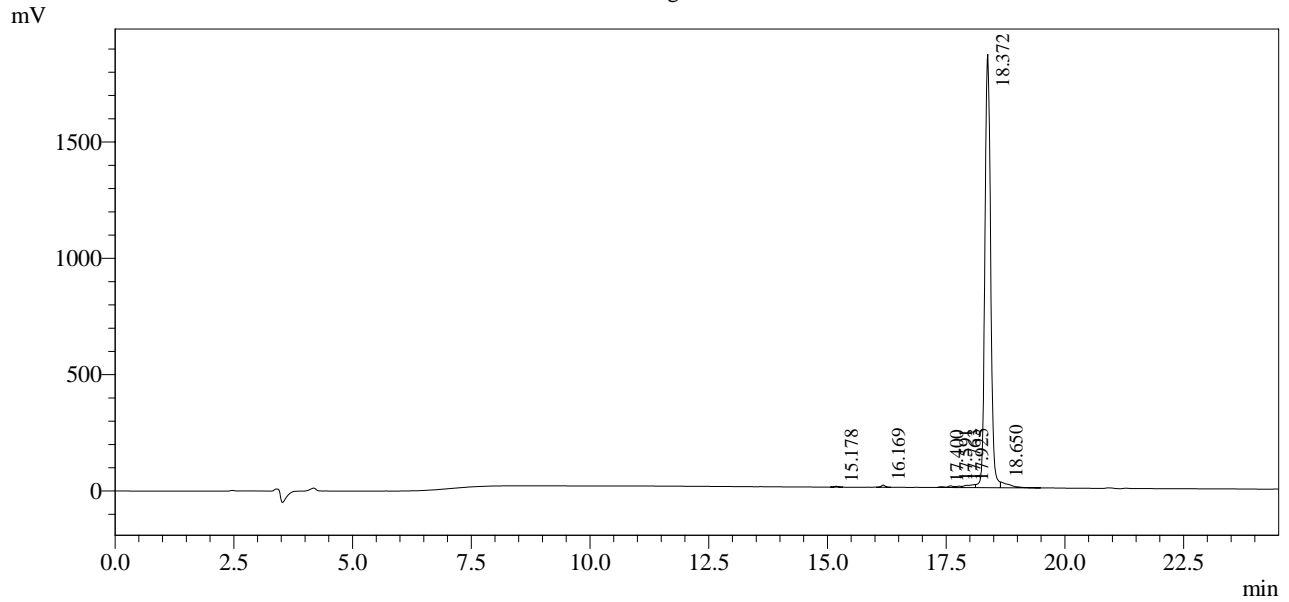

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.178	21181	3780	0.129
2	16.169	55925	9310	0.340
3	17.400	23740	3248	0.144
4	17.591	50605	7469	0.308
5	17.763	41343	5869	0.252
6	17.925	169727	9430	1.033
7	18.372	15755420	1862148	95.867
8	18.650	316810	24501	1.928
Total		16434751	1925755	100.000