


Positive

### MS Spectrum

Intensity

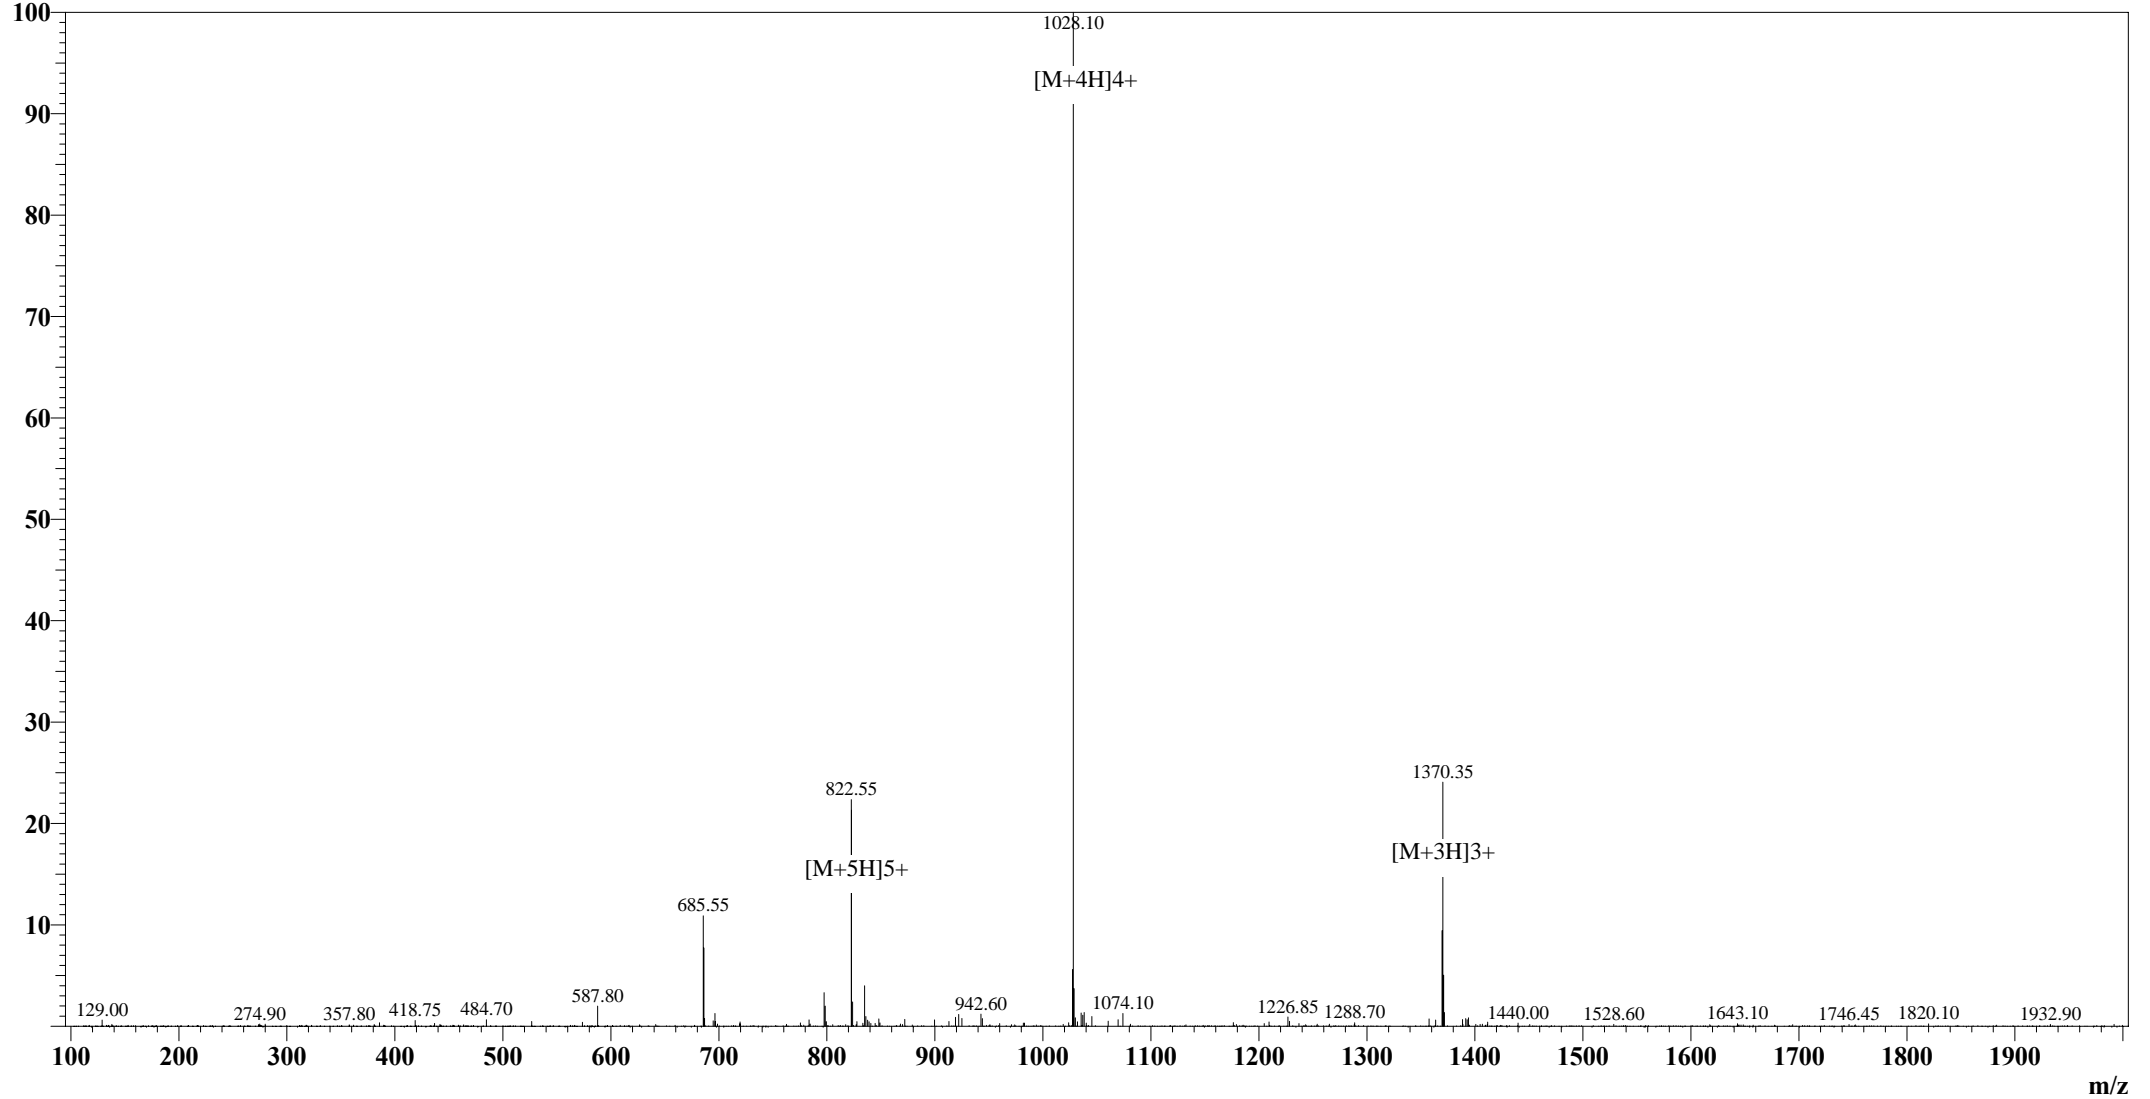

#### Sample Information

User : Grace  
Date Acquired : 07/22/2009 11:17:34  
Sample Name : PTH(1-34),bovine  
Cat No. : RP10364  
Lot No. : CD19907  
Injection Volum : 1.000µL  
Theoretical MW : 4108.73  
Observed MW : 4108.40

Interface : ESI  
Nebulizing Gas Flow : 1.50 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH