


Positive

MS Spectrum

Intensity

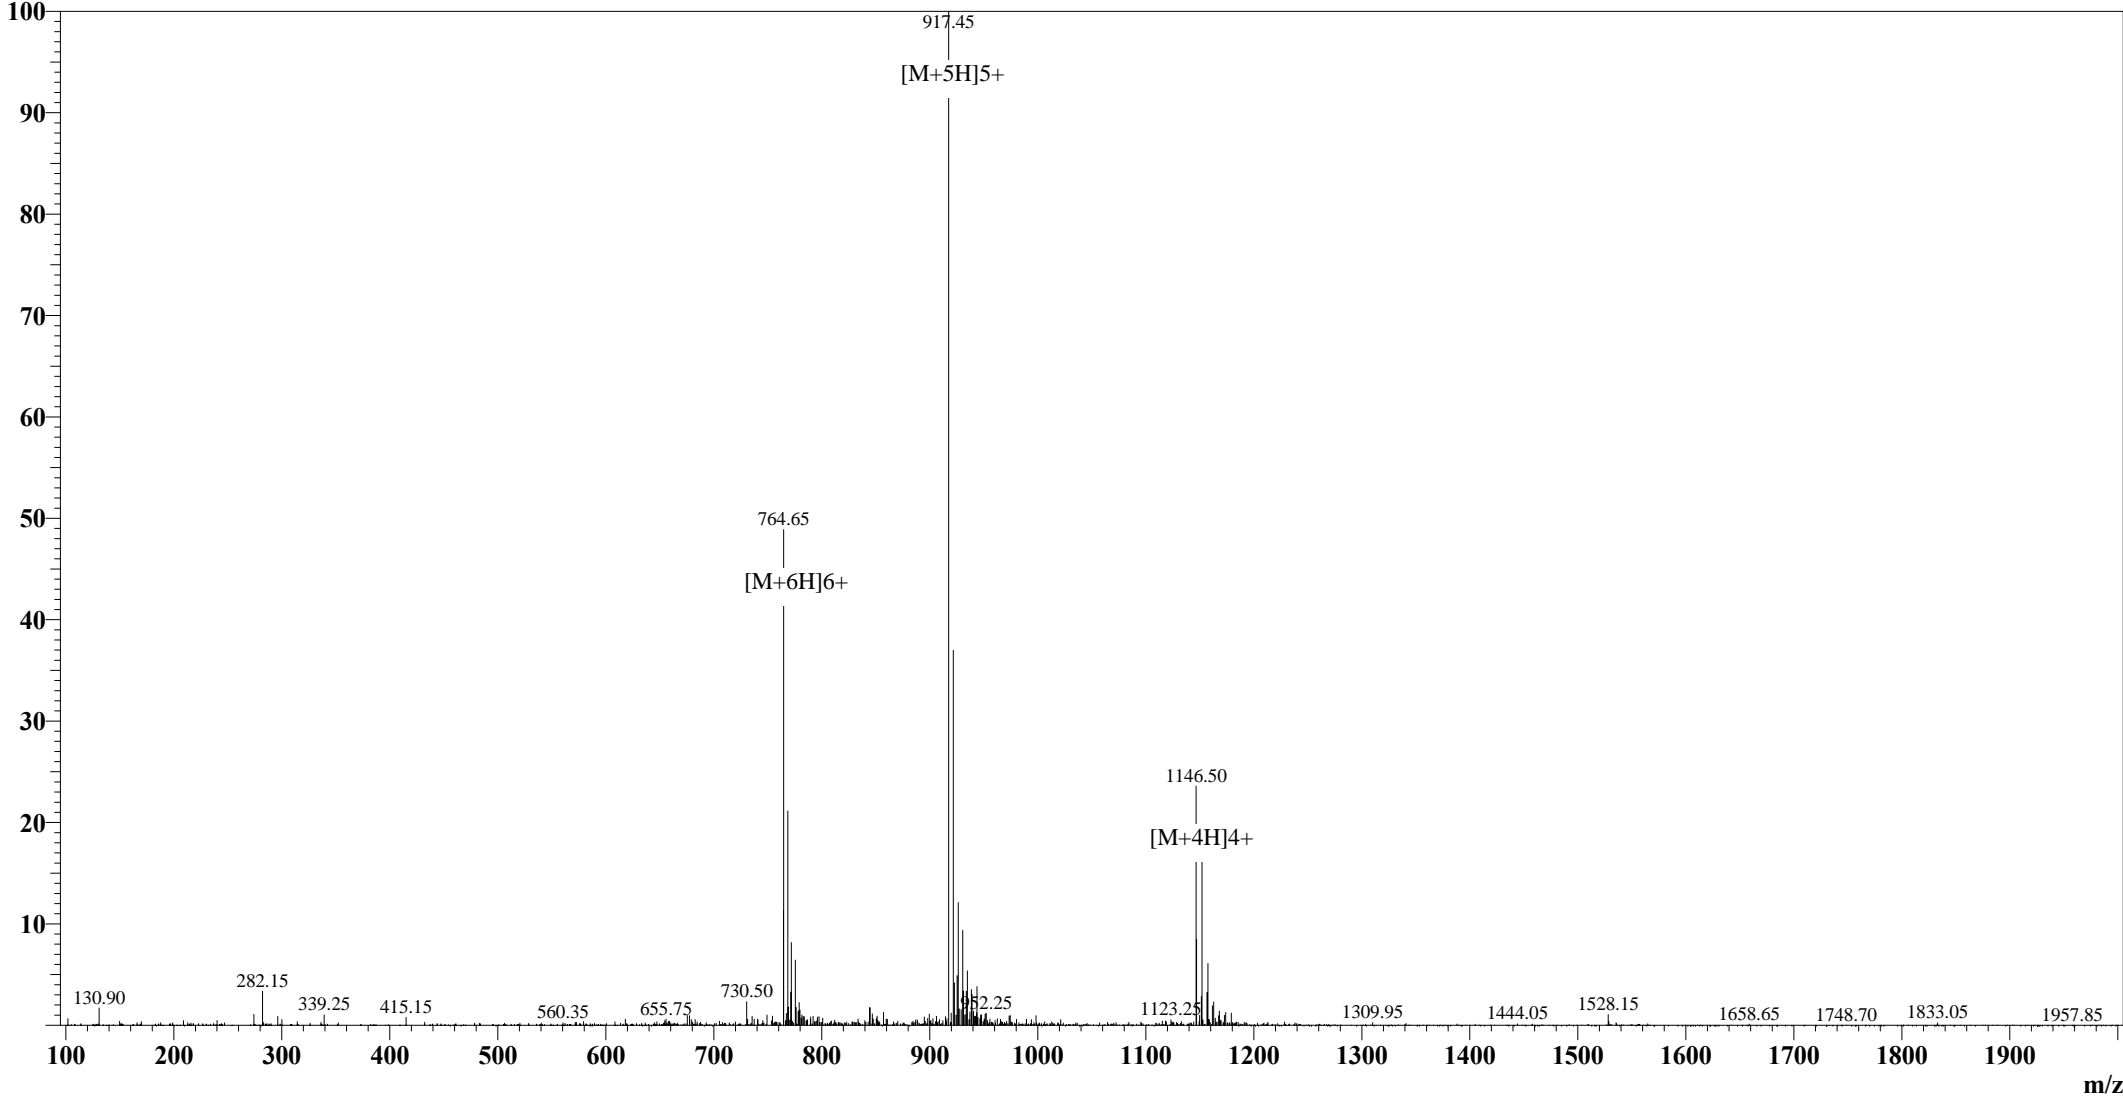

Sample Information

User : Grace  
Date Acquired : 07/30/2009 9:02:58  
Sample Name : ACTH (1-39), rat  
Cat No. : RP11305  
Lot No. : CC11907  
Injection Volum : 1.000µL  
Theoretical MW : 4582.50  
Observed MW : 4582.25

Interface : ESI  
Nebulizing Gas Flow : 1.50 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH