

Sample Name :c-Myc Peptide
 Cat. No. :RP11731
 Lot. No. :88606001012610ZW

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

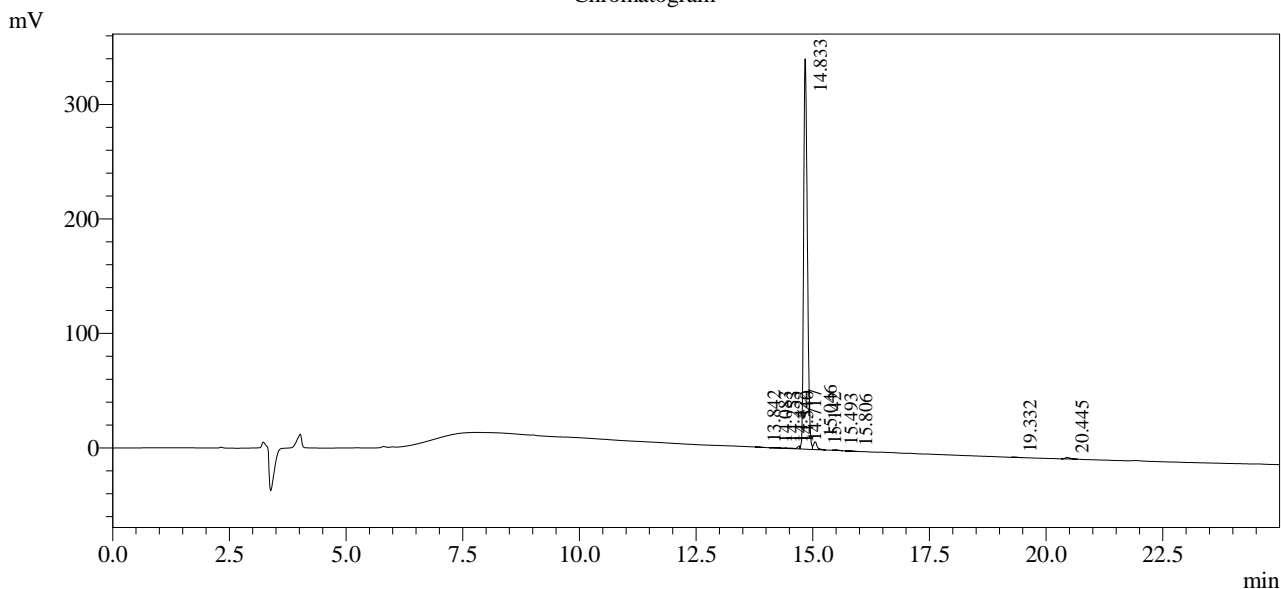

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	13.842	742	147	0.038
2	14.083	380	4	0.019
3	14.253	1936	286	0.099
4	14.422	3016	528	0.154
5	14.540	2791	470	0.143
6	14.717	9695	2528	0.496
7	14.833	1882413	340993	96.362
8	15.046	33985	6842	1.740
9	15.142	2506	742	0.128
10	15.493	3557	644	0.182
11	15.806	1569	290	0.080
12	19.332	1188	204	0.061
13	20.445	9710	1355	0.497
Total		1953487	355032	100.000