


Positive MS Spectrum

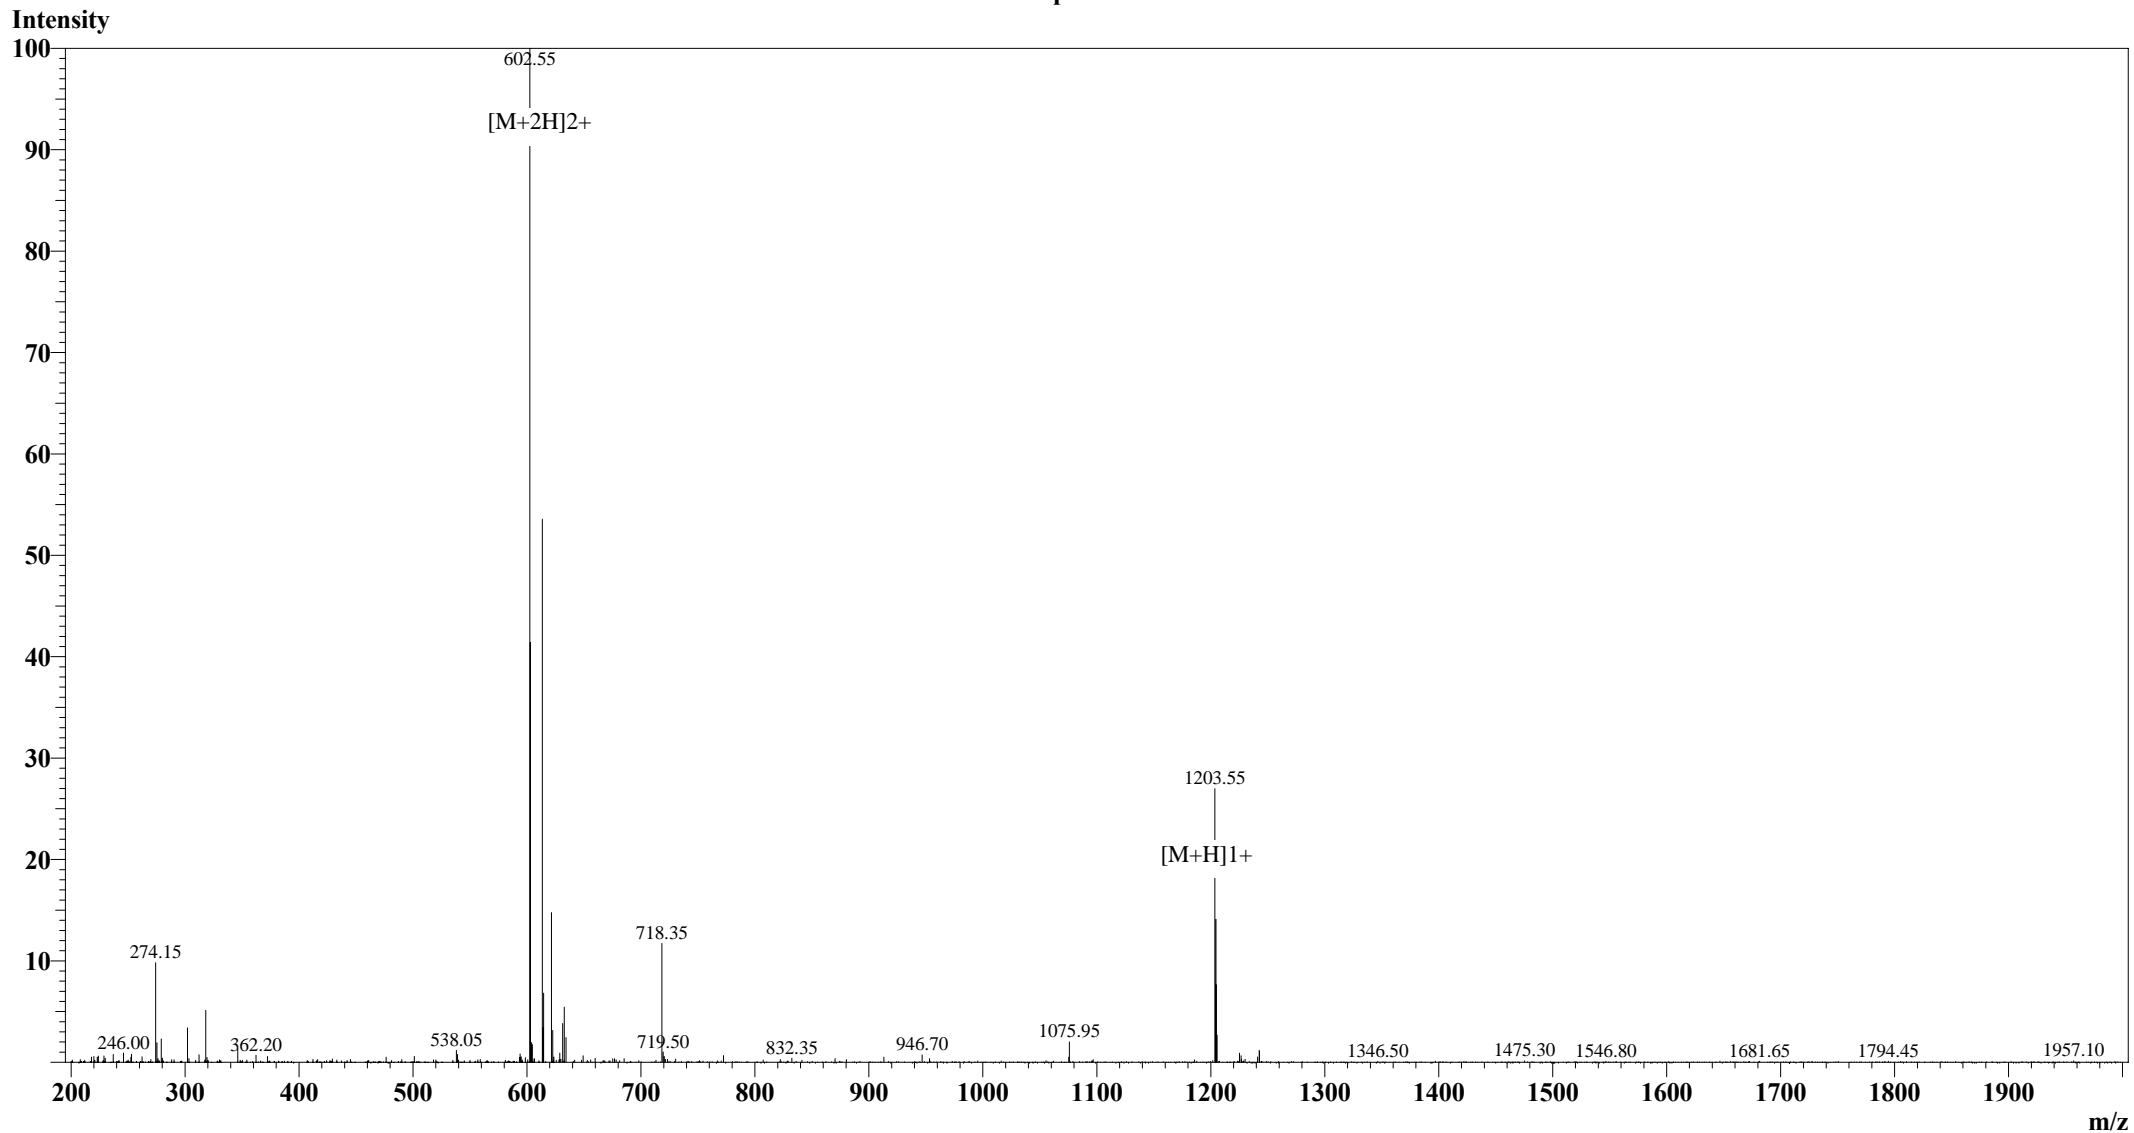

Sample Information

User : Grace
Date Acquired : 01/27/2010 14:35:32
Sample Name : c-Myc Peptide
Cat No. : RP11731
Lot No. : 88606001012610ZW
Injection Volum : 1.000µL
Theoretical MW : 1203.30
Observed MW : 1203.10

Interface : ESI
Nebulizing Gas Flow : 4.21 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH