


Positive

MS Spectrum

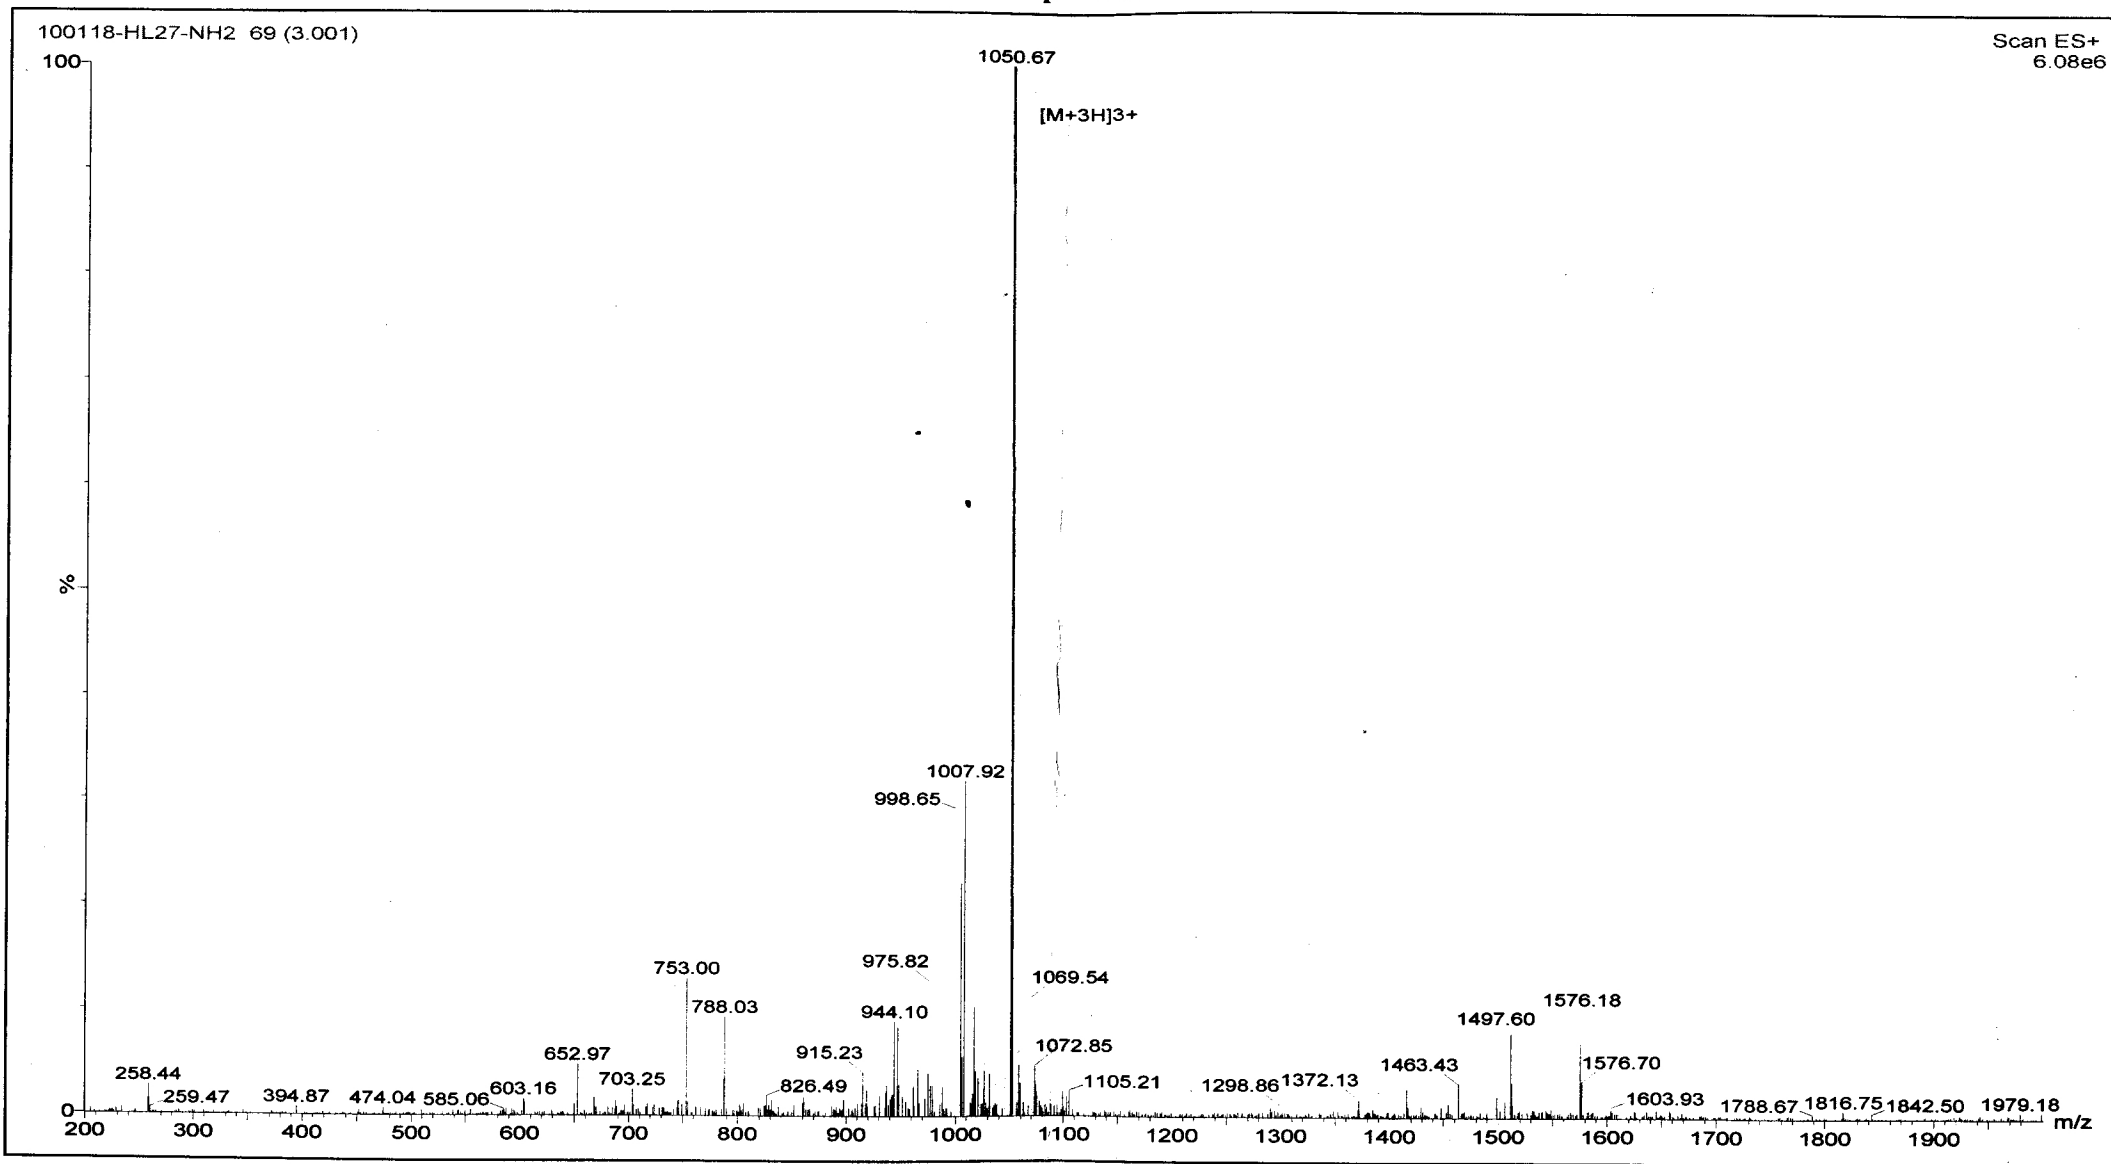

Sample Information Item

Date and Time : 18-Jan-2010 09:35:45  
Sample Name : PACAP(1-27) , human, ovine, rat  
Lot. No : 83177001011210ZJ  
MW : 3147.68

Probe: ESI  
Cone: 50V  
Capillary: 3.00KV  
Extractor: 5V

Gas Flow: 350L/hr  
T.Flow: 0.2ml/min  
Desovation Temp: 350°C  
B.conc: 50%H2O/50%ACN