

Sample Name : Arg-Gly-Asp-Cys
 Cat. No. :RP10860
 Lot. No. :87303001011110WJ

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
31.00	Pumps	Pump A B.Conc	95	
31.01	Pumps	Pump A B.Conc	5	
40.00	Pumps	Pump A B.Conc	5	
40.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

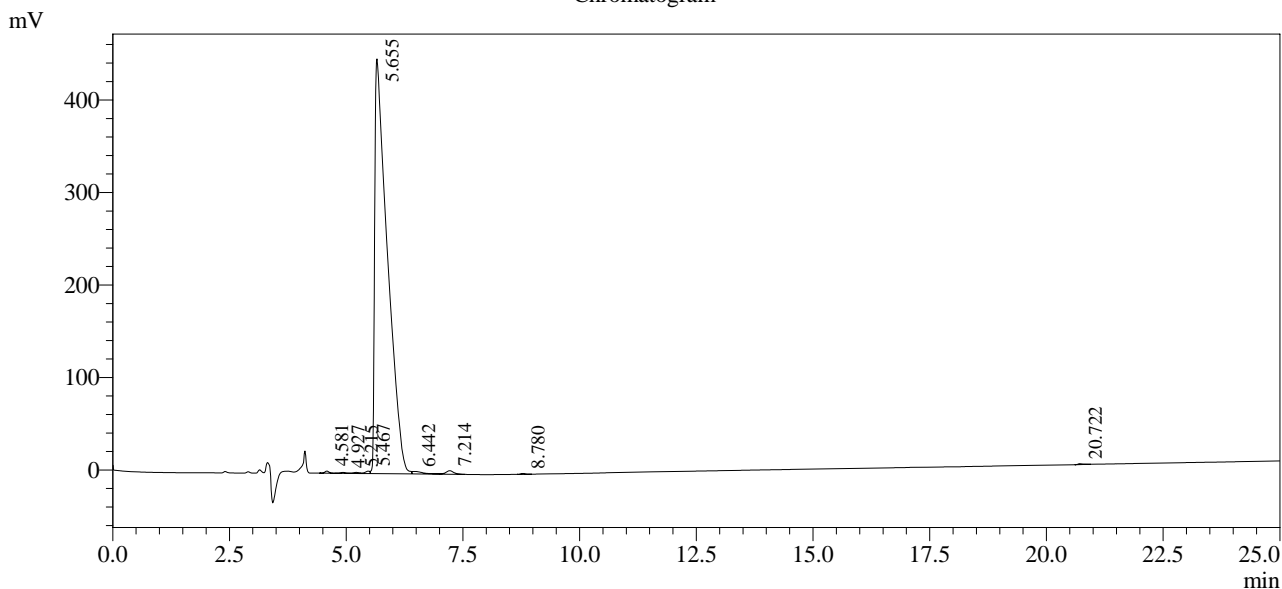

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	4.581	13773	2267	0.159
2	4.927	10014	952	0.116
3	5.215	10119	1179	0.117
4	5.467	19508	2562	0.225
5	5.655	8513413	448474	98.198
6	6.442	45137	2721	0.521
7	7.214	44941	3852	0.518
8	8.780	5200	834	0.060
9	20.722	7530	1060	0.087
Total		8669635	463901	100.000