


Positive MS Spectrum

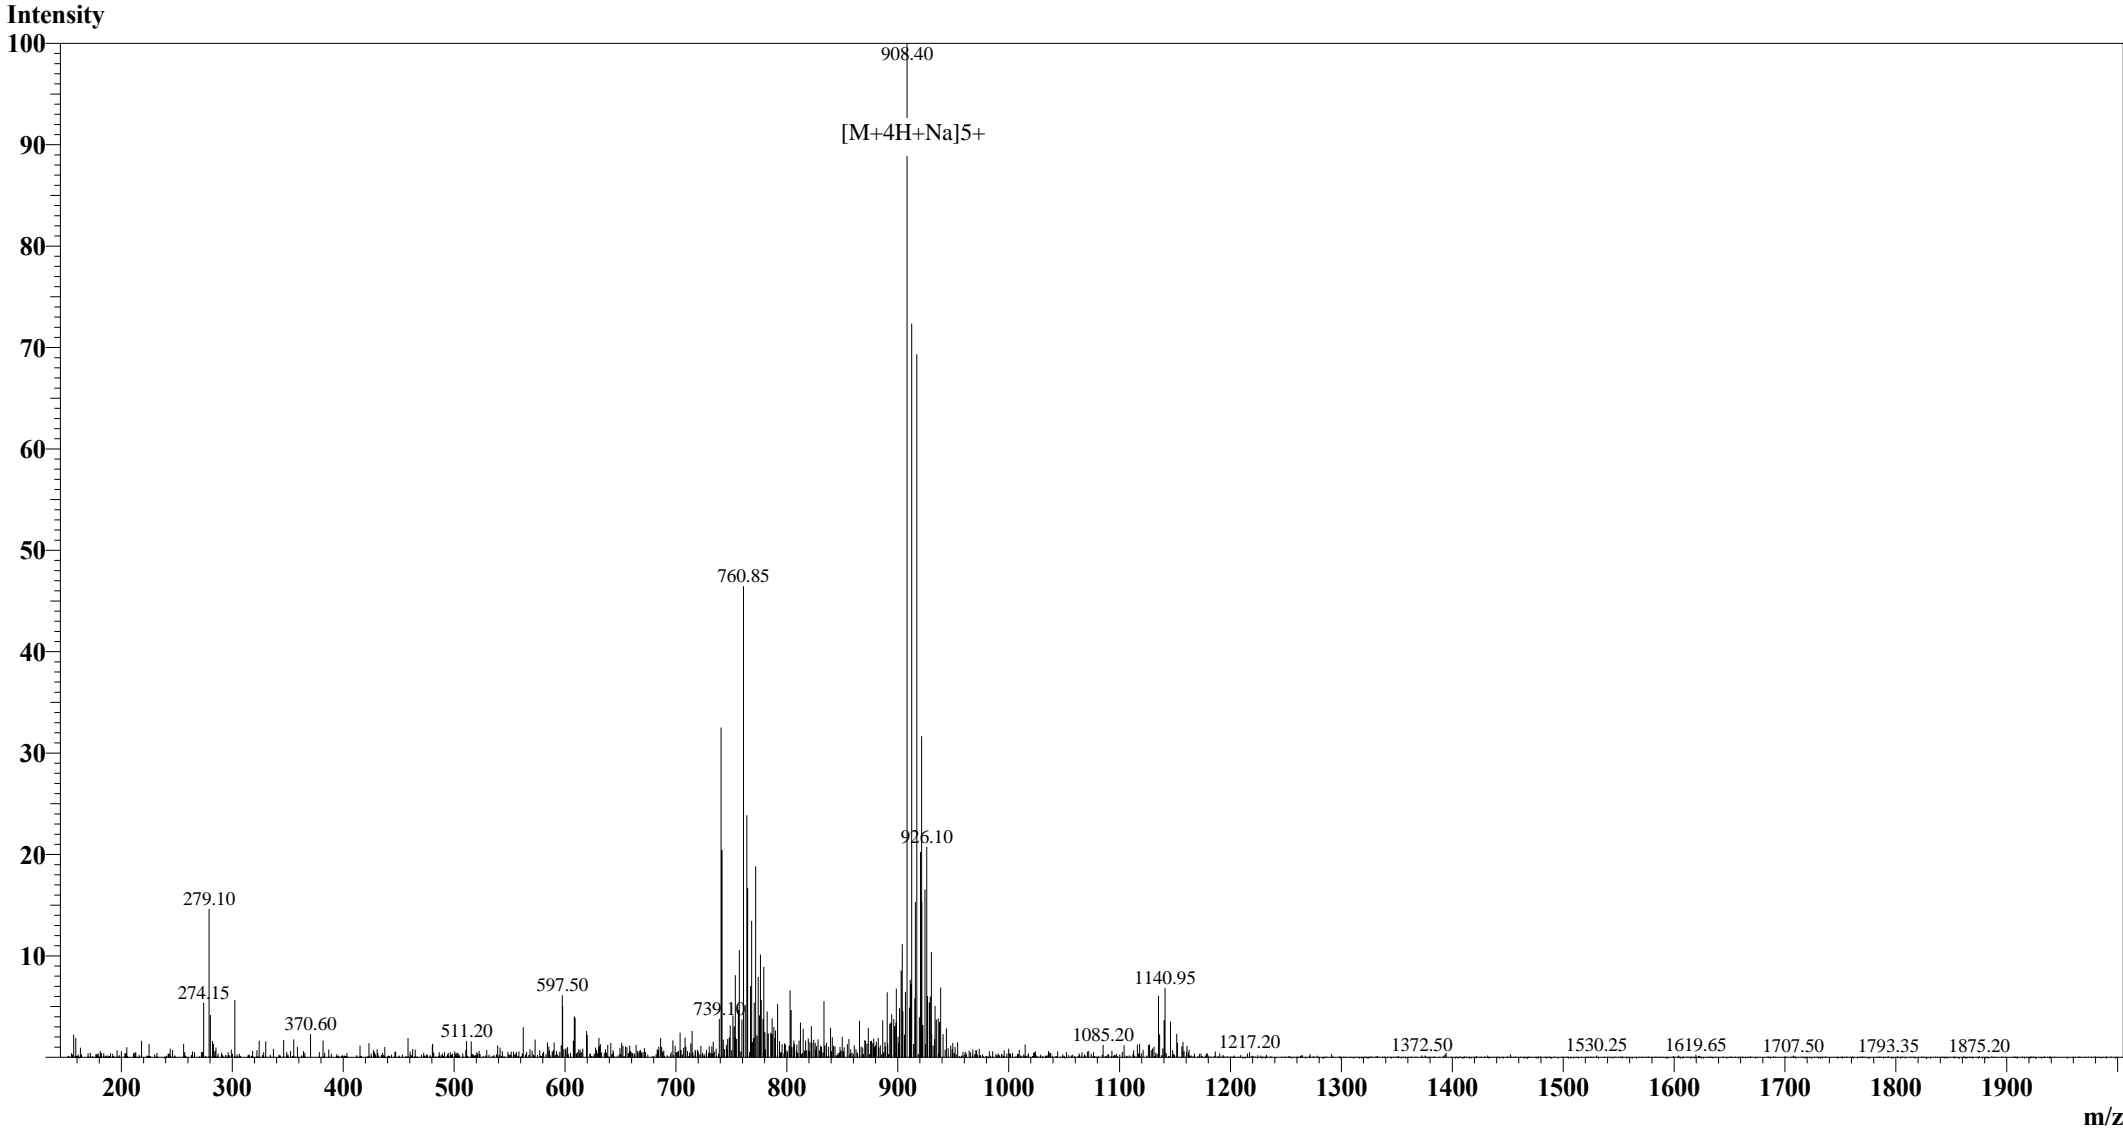

**Sample Information**  
User : Grace  
Date Acquired : 12/04/2009 20:09:20  
Sample Name :  $\beta$ -Amyloid (1-42), human  
Cat No. : RP10017  
Lot No. : 78425001091009XB  
Injection Volum : 1.000 $\mu$ L  
Theoretical MW : 4514.10  
Observed MW : 4515.00

Interface : ESI  
Nebulizing Gas Flow : 1.50 L/min  
CDL Temp : 250 $^{\circ}$ C  
CDL Volt : -25.0V  
Block Temp : 200 $^{\circ}$ C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H<sub>2</sub>O/50%MeOH