


Positive

### MS Spectrum

Intensity

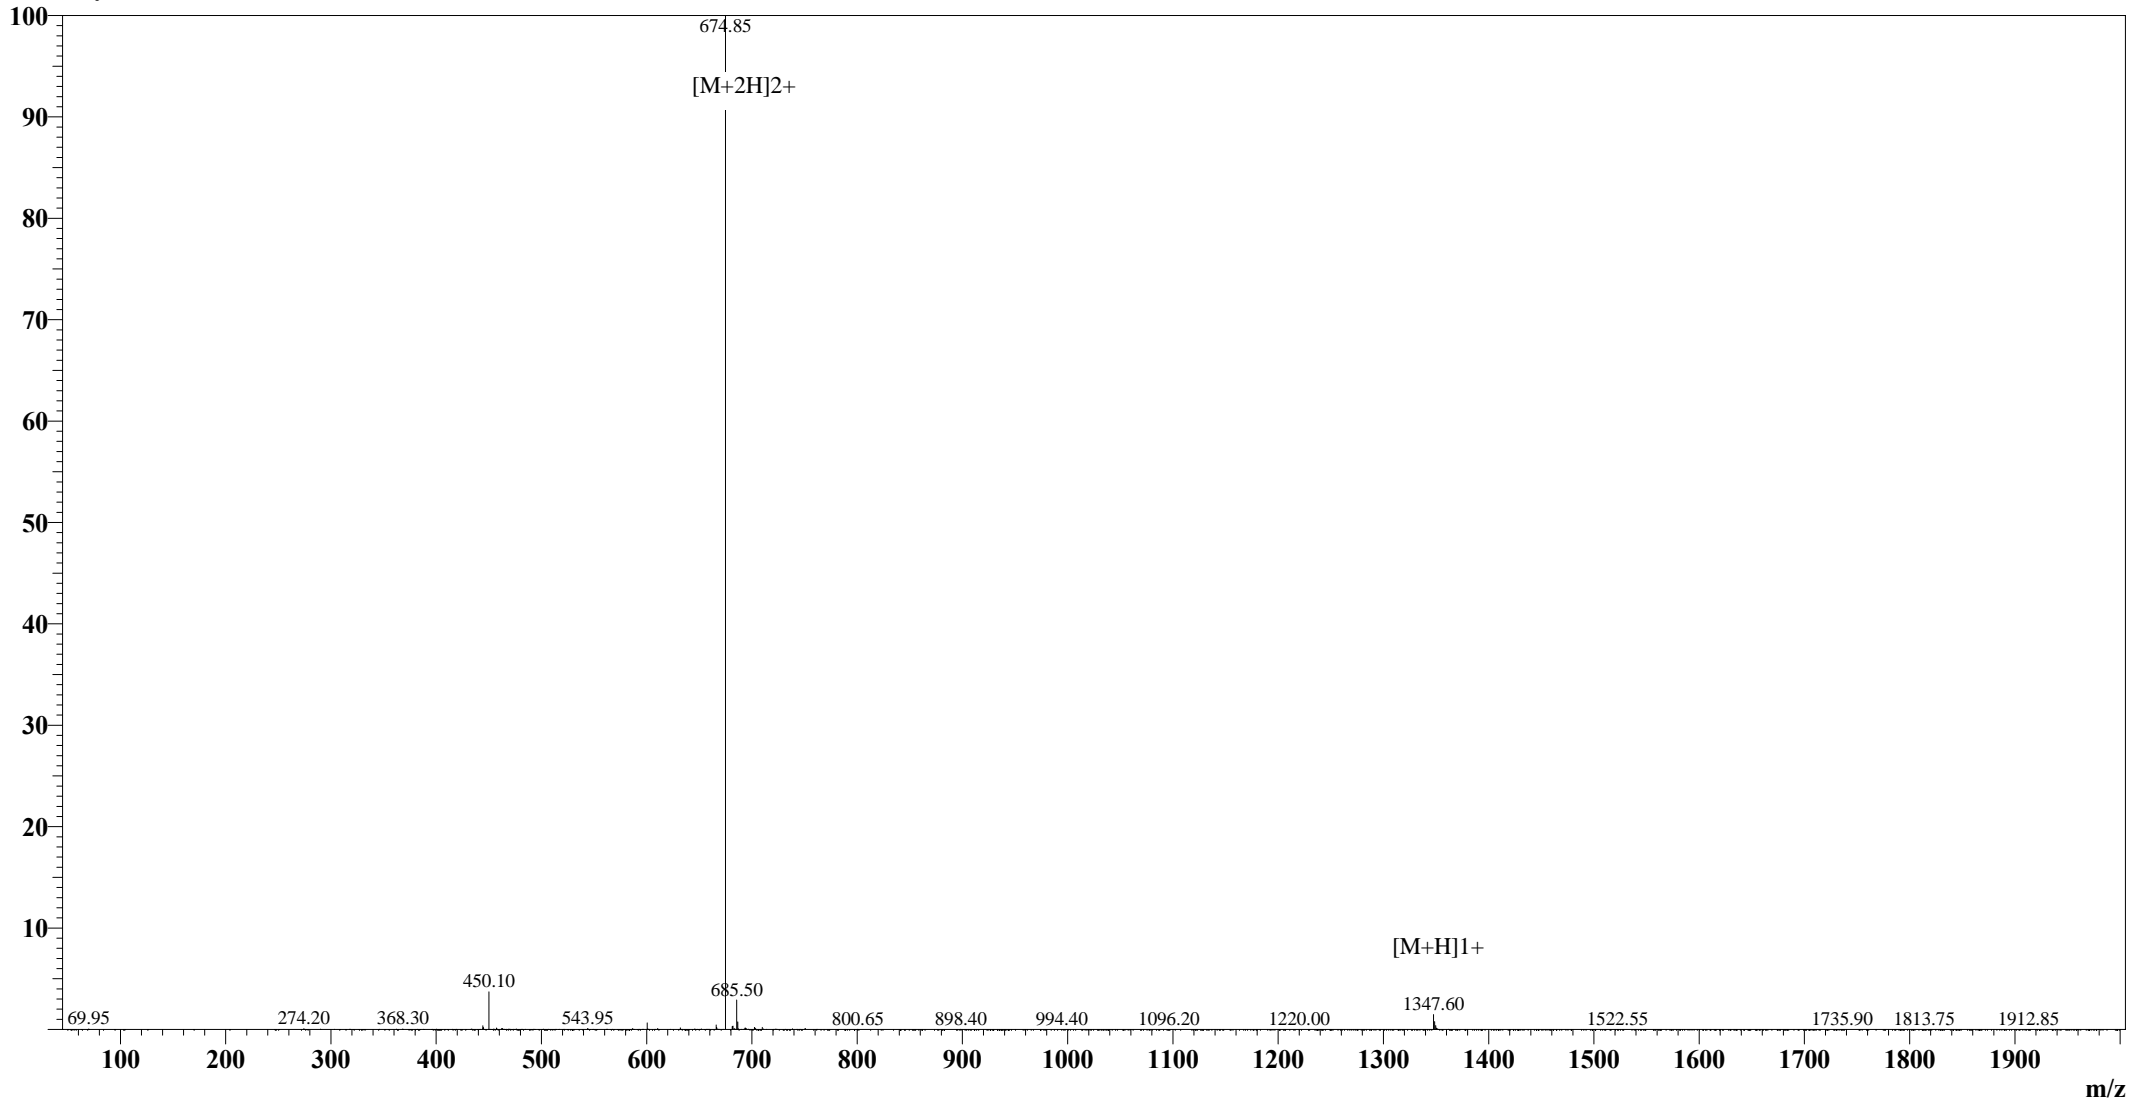

#### Sample Information

User : Grace  
Date Acquired : 02/04/2009 10:00:13  
Sample Name : Substance P  
Cat No. : RP10178  
Lot No. : CC01902  
Injection Volum : 1.000µL  
Theoretical MW : 1347.63  
Observed MW : 1347.70

Interface : ESI  
Nebulizing Gas Flow : 1.50 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias : +4.5kv  
Detector : 1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH