


MS Spectrum

Positive

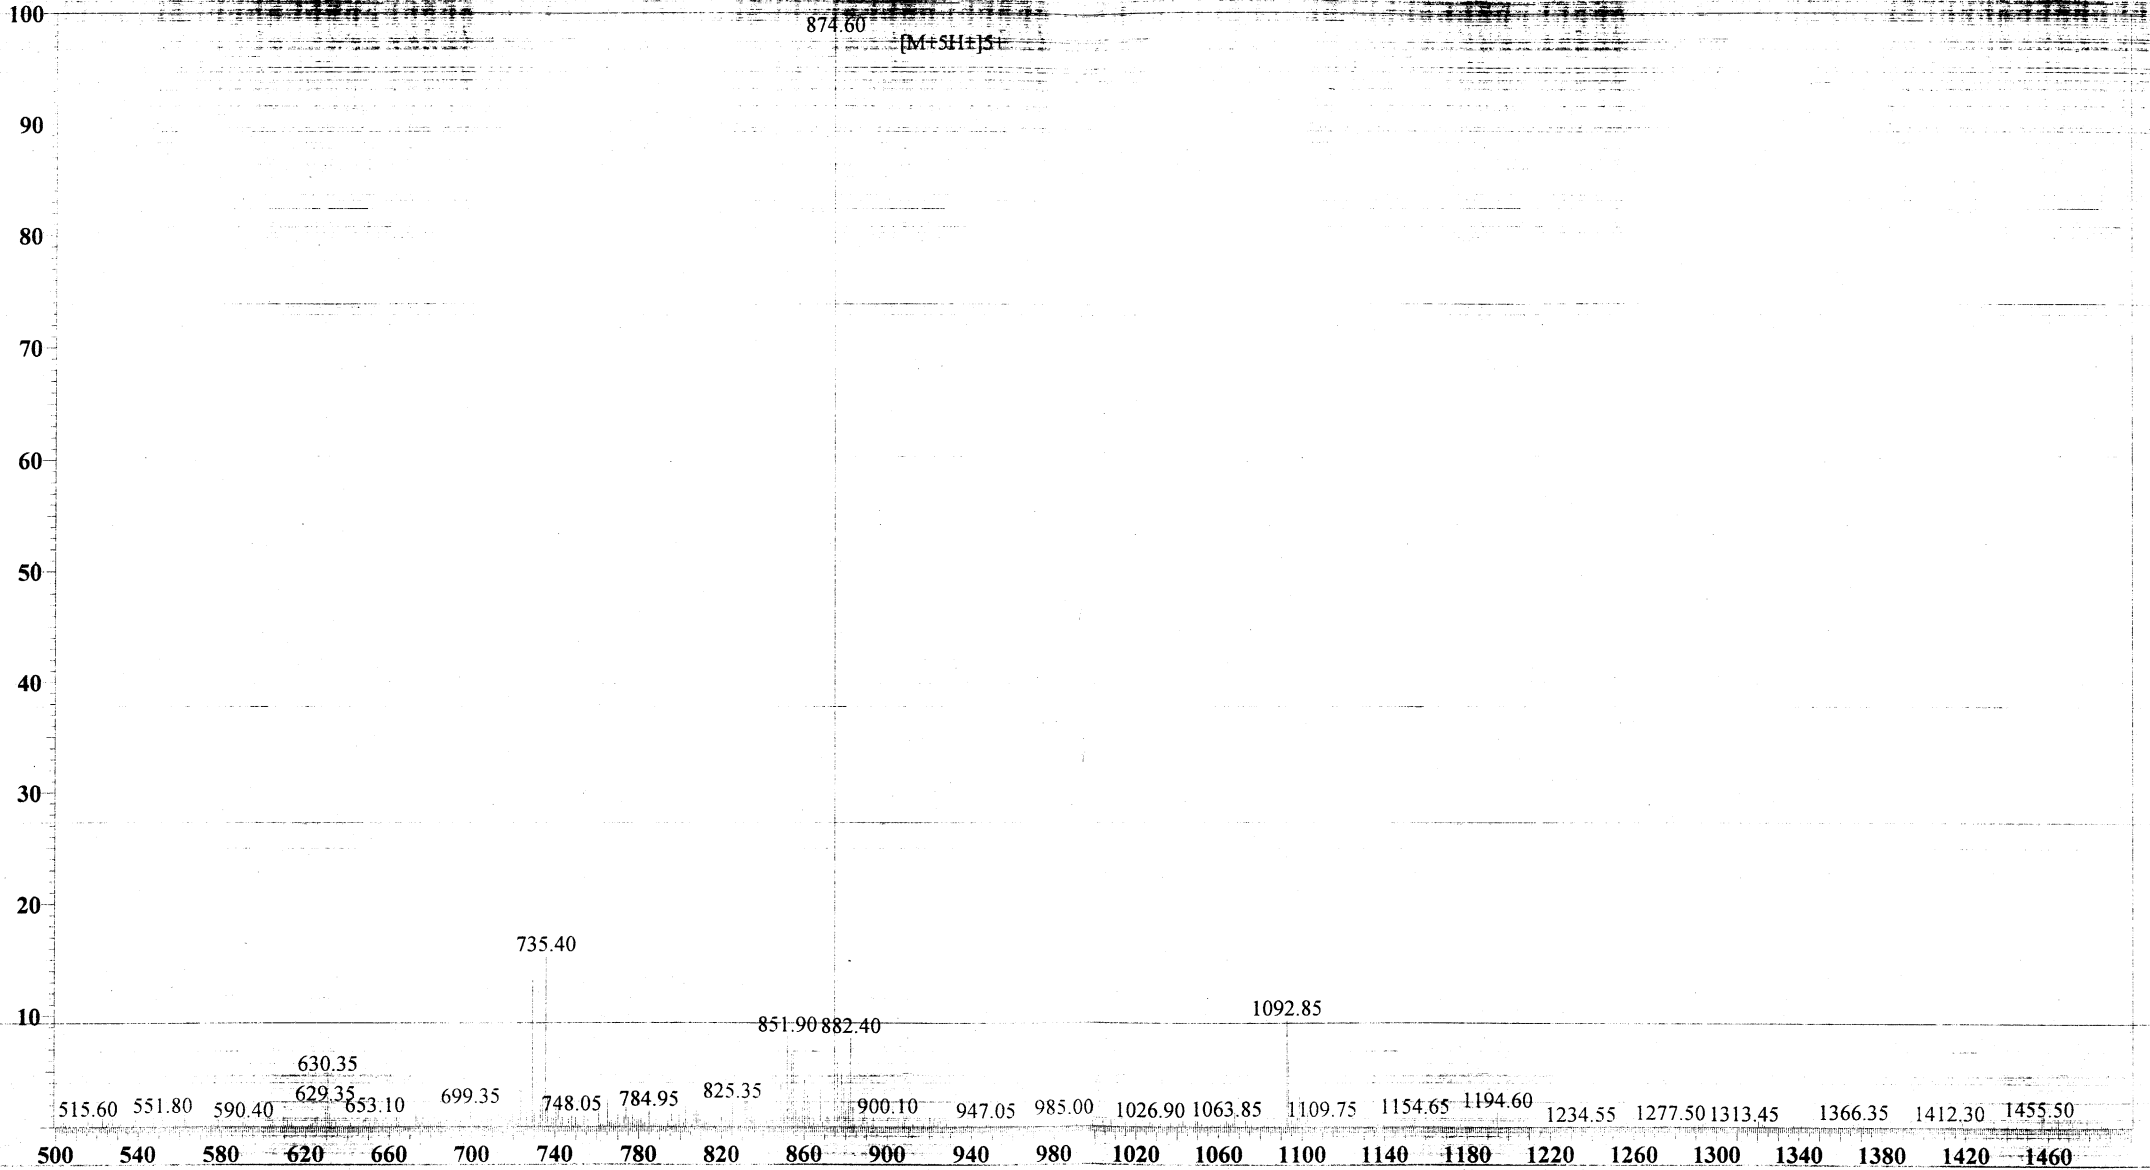

Sample Information Item
Date and Time : 2005-3-11 13:06:56
User : FJS
Sample : RP10214(TI-40)
Inj. Volume : 1.000
MW : 4367.24

Cat. No.: RP10214
Lot No.: PJ00415506

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%AGN

m/z