


MS Spectrum

Positive

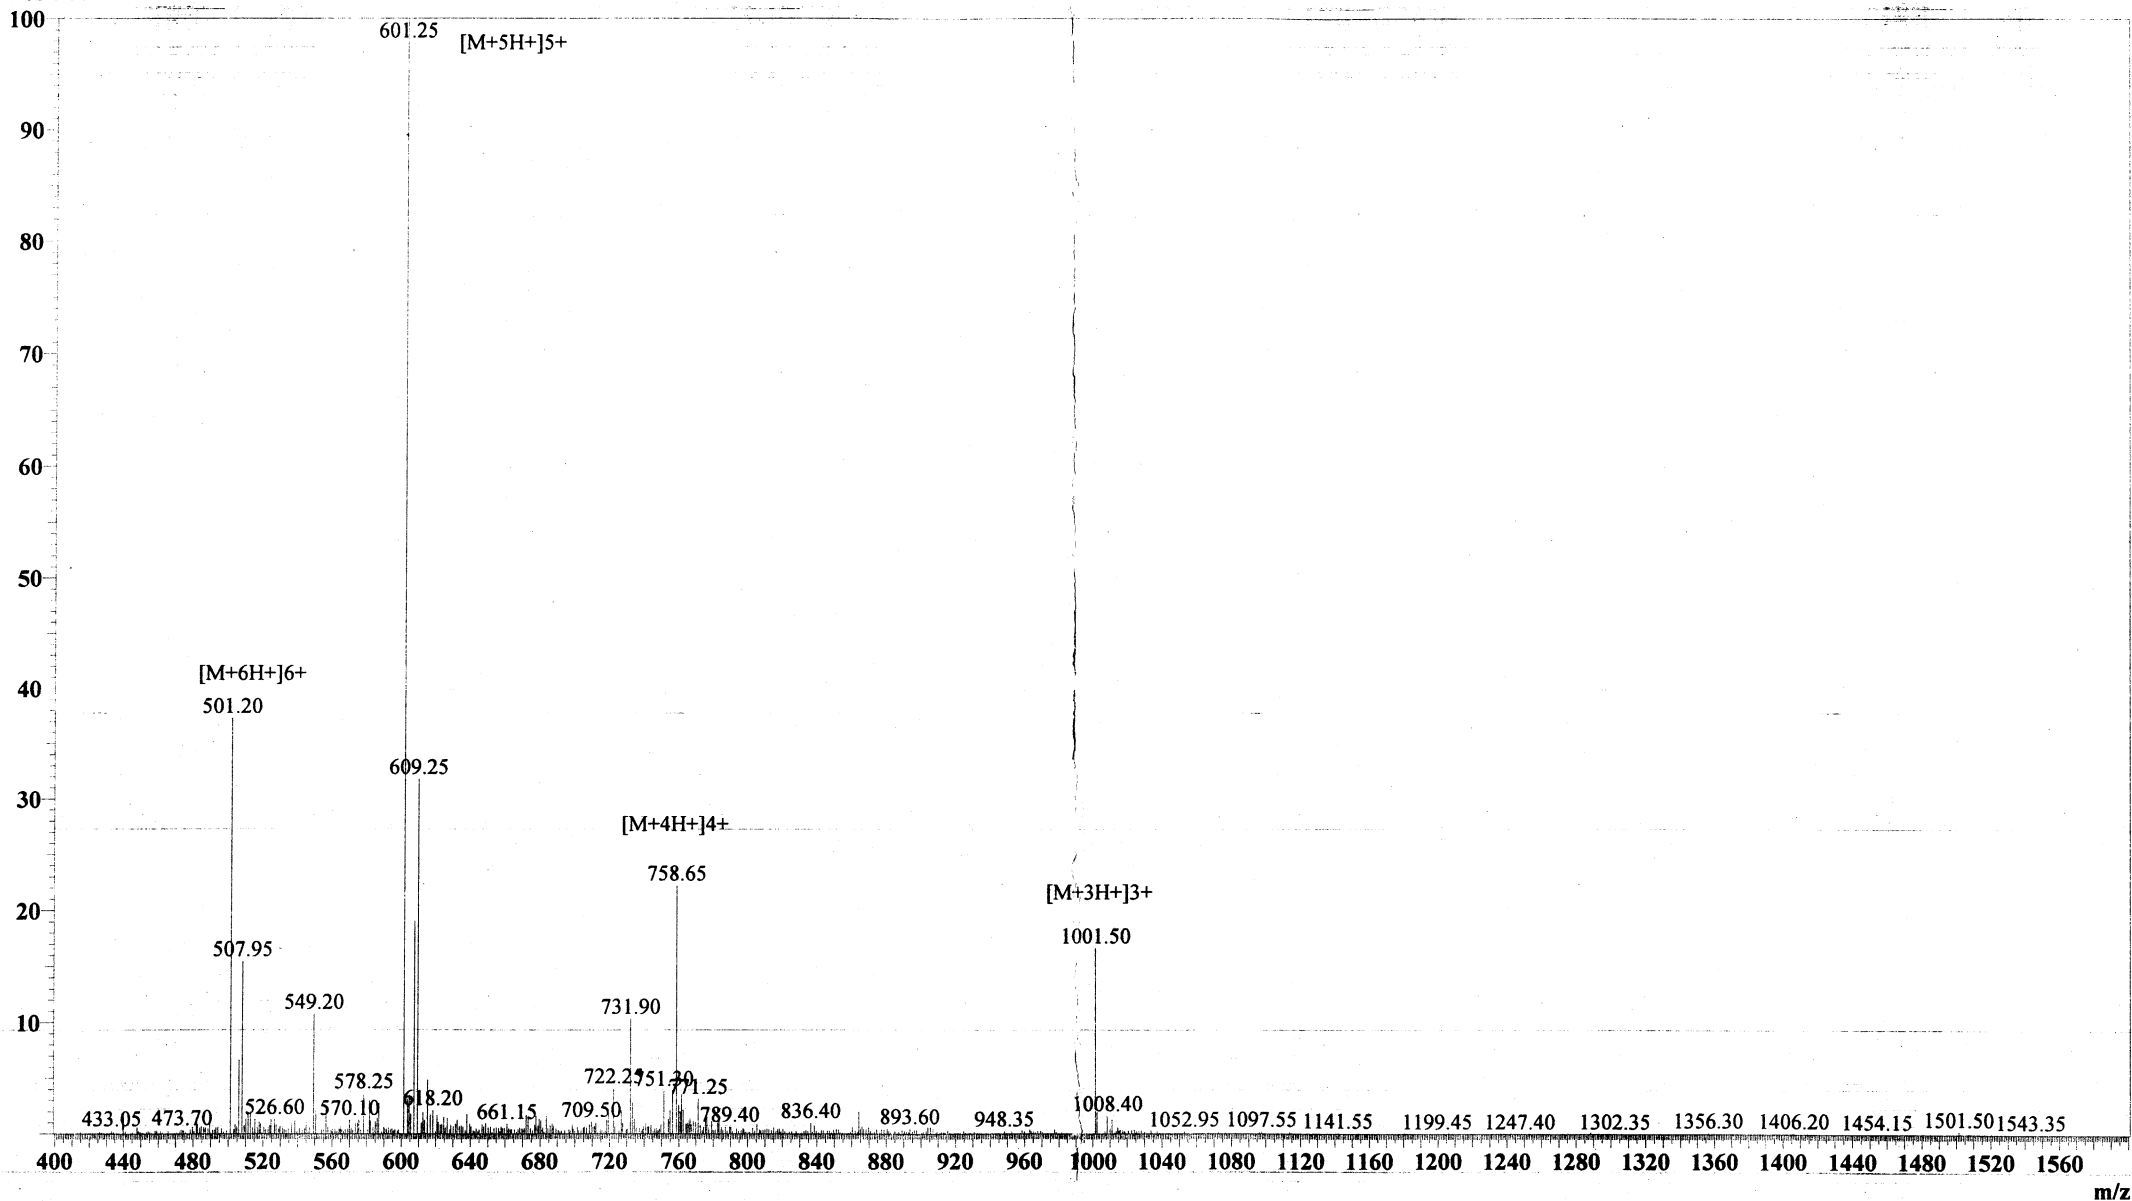

Sample Information Item

Date and Time : 2005-3-5 17:16:44
User : xie
Sample : RP10488 PY-24-NH2
Inj. Volume : 1.000
MW : 3000.46

Cat. No.: RP10488

Lot No.: PX00107503

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN

m/z