


MS Spectrum

Positive

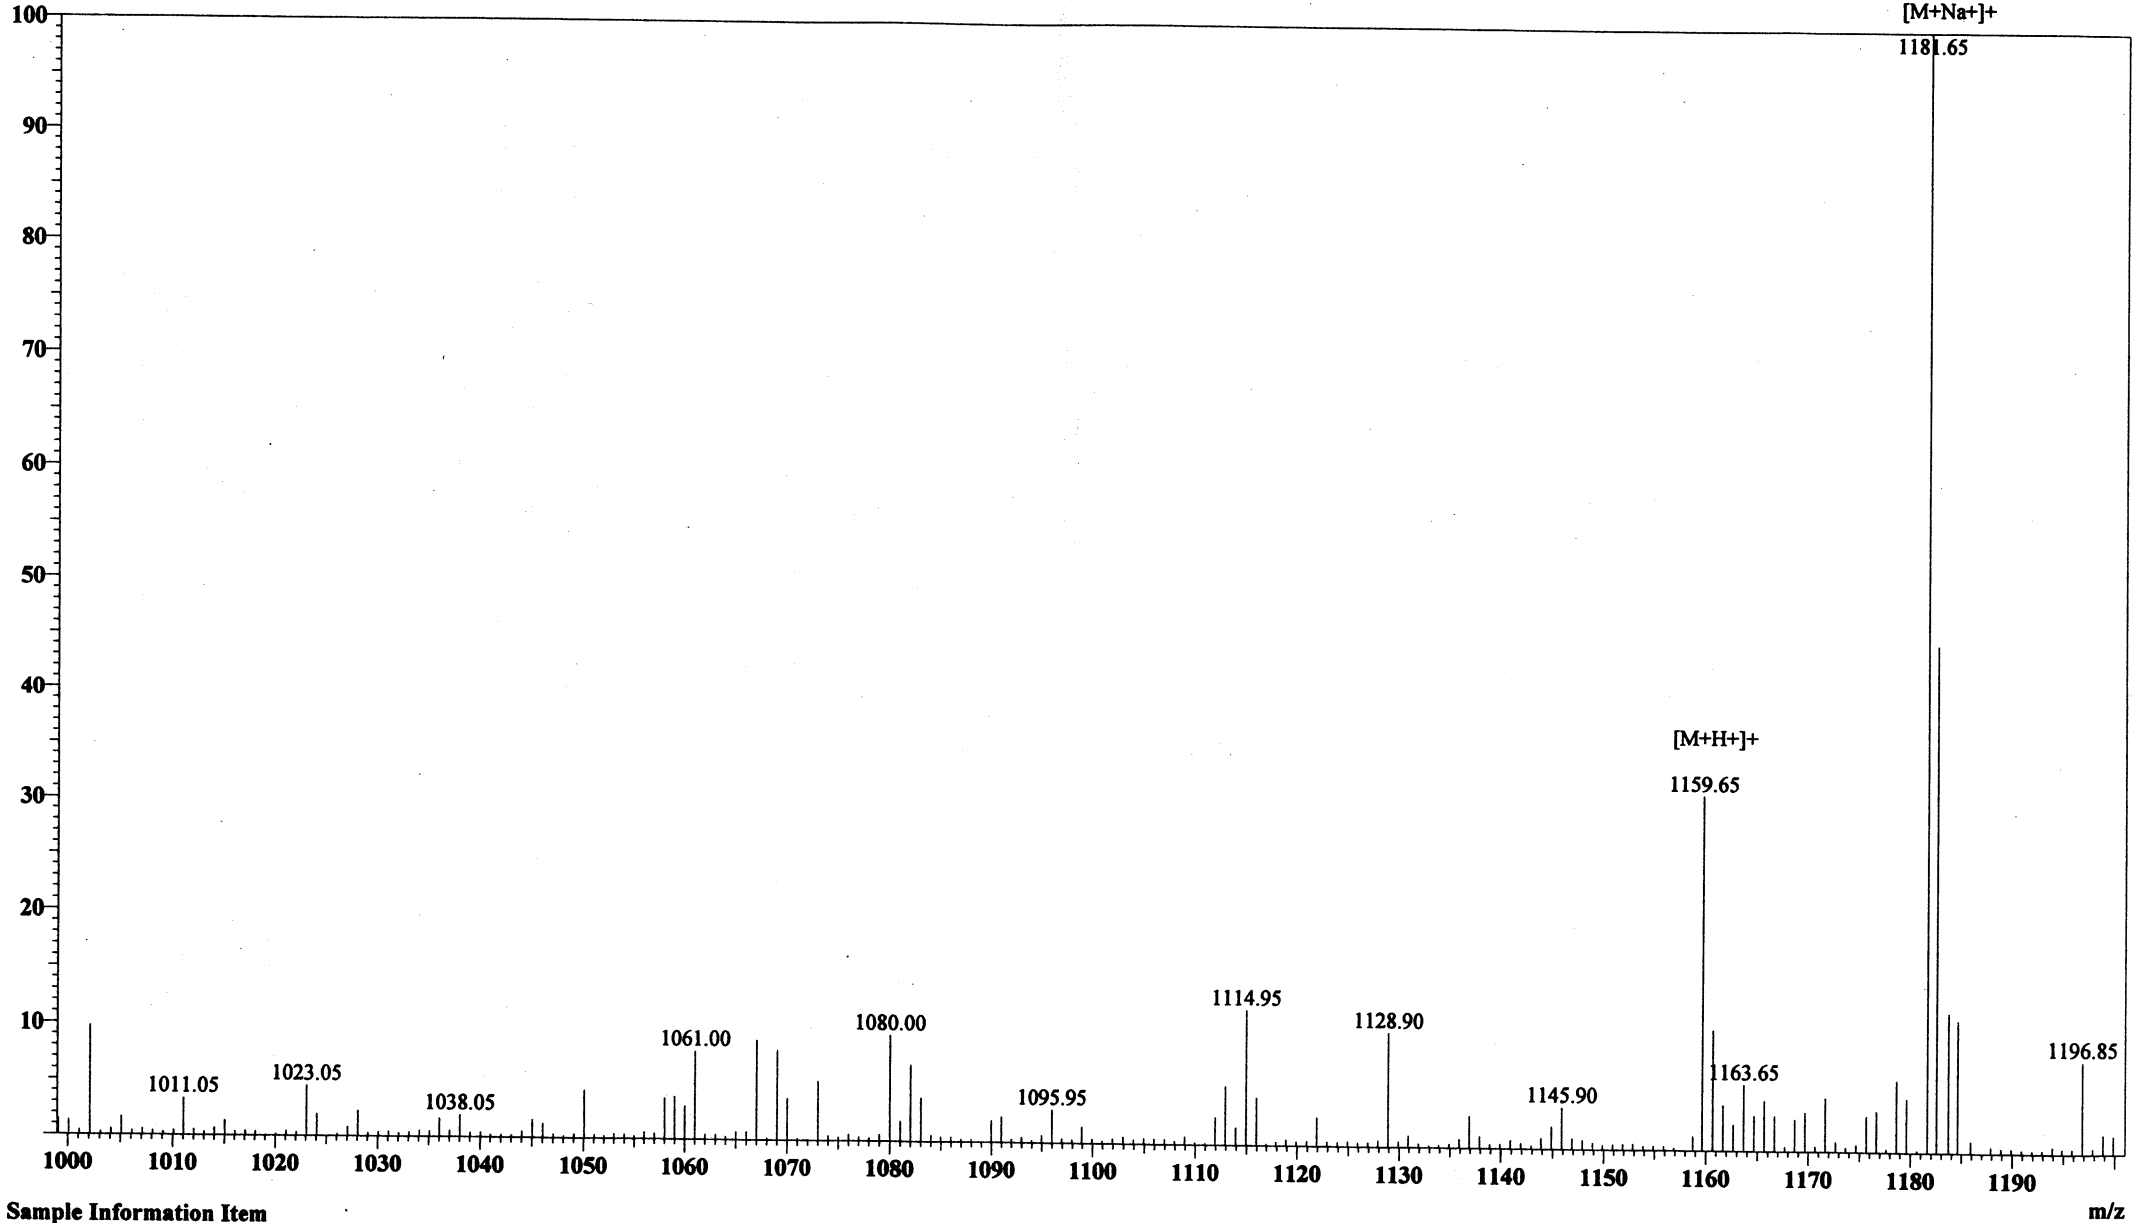

Sample Information Item

Date and Time : 2005-5-12 15:47:46  
User : FJS  
Sample : RP11319 PET-10-NH2  
Inj. Volume : 1.000  
MW : 1159.28

Cat. No.: RP11319  
Lot No.: PJ00130505

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN