


Positive MS Spectrum

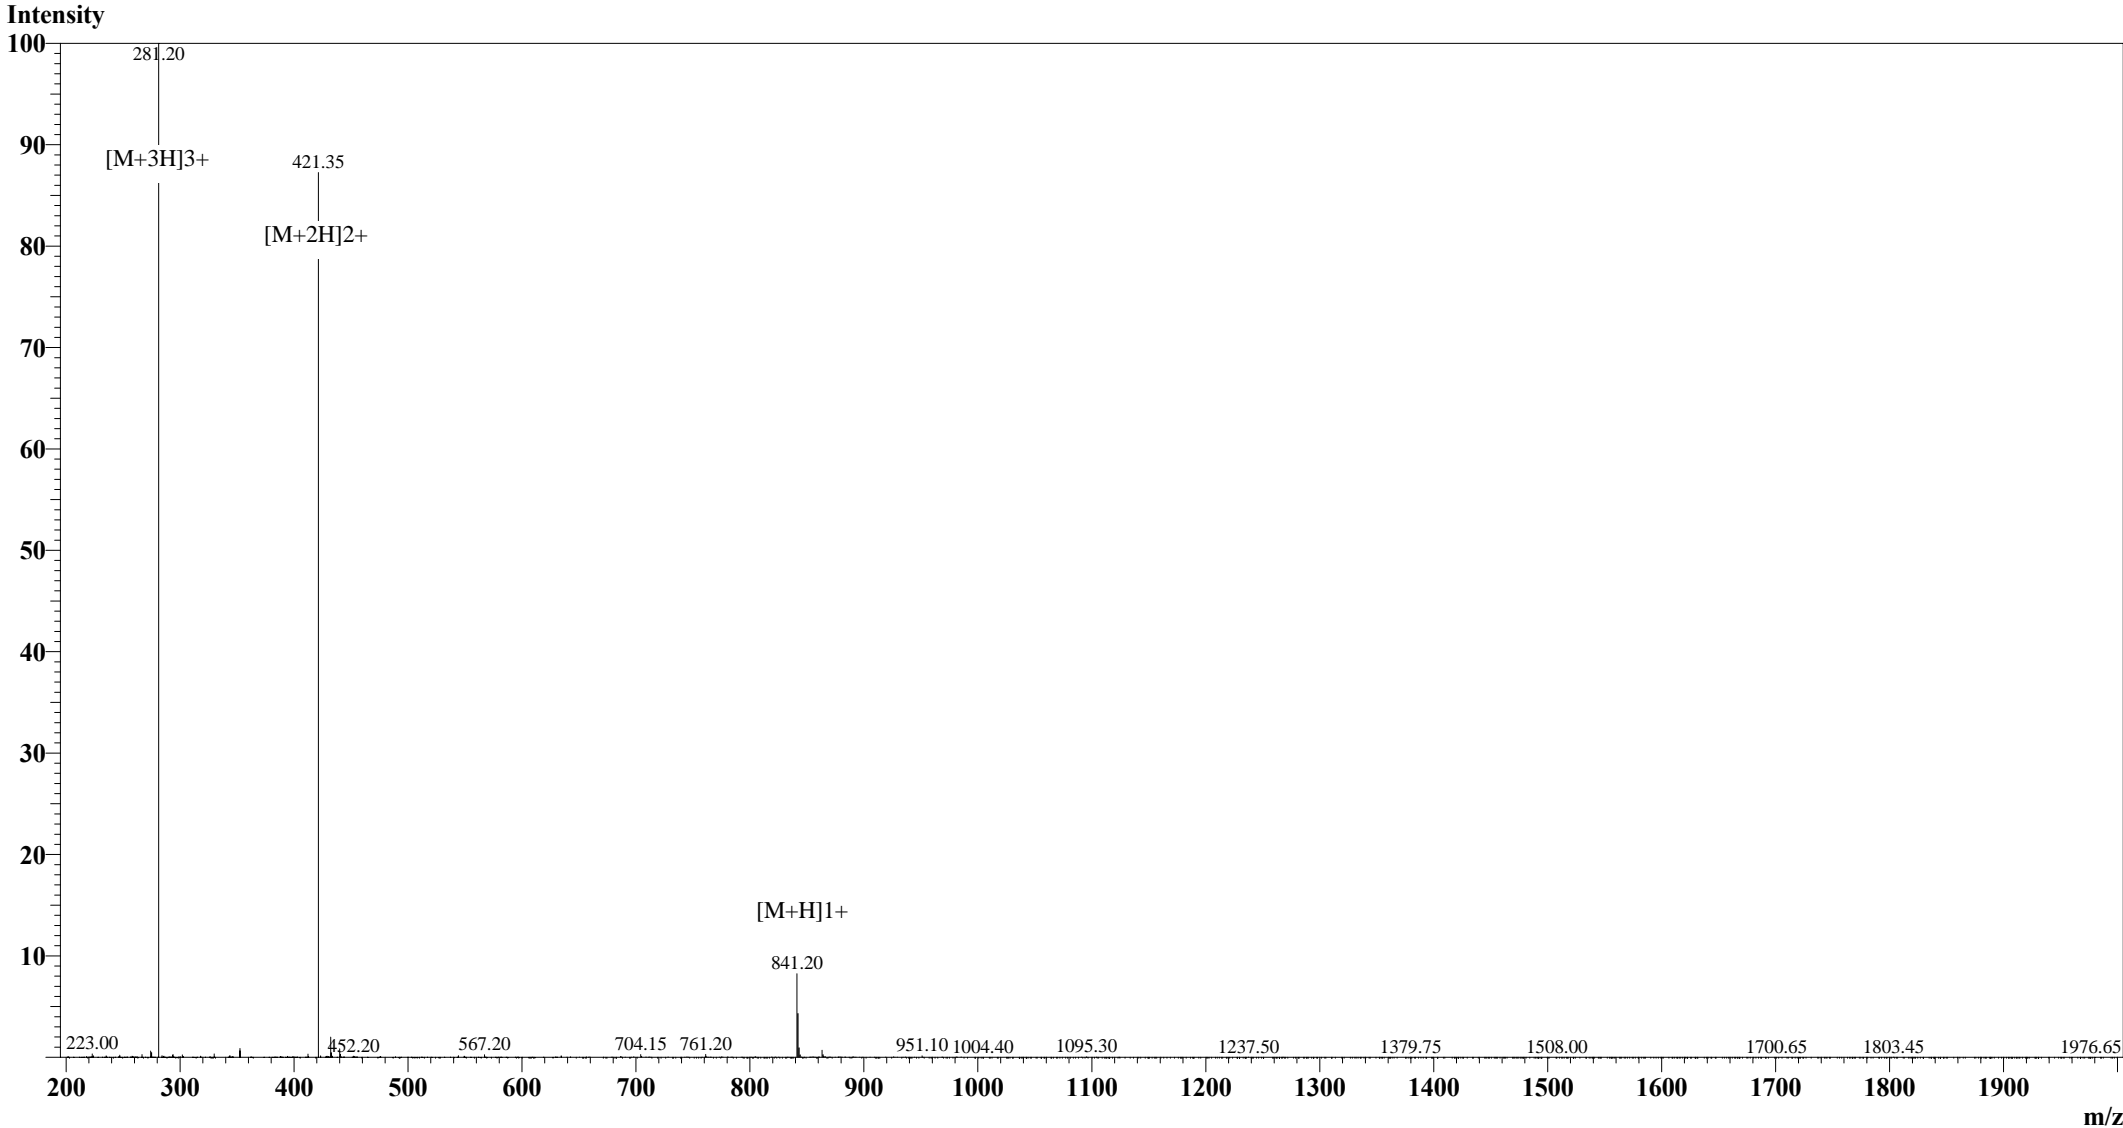

Sample Information
User : Grace
Date Acquired : 09/08/2009 22:19:16
Sample Name : Hexa-His
Cat No. : RP11737
Lot No. : CB03909
Injection Volum : 1.000µL
Theoretical MW : 840.85
Observed MW : 840.20

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH