


MS Spectrum

Positive

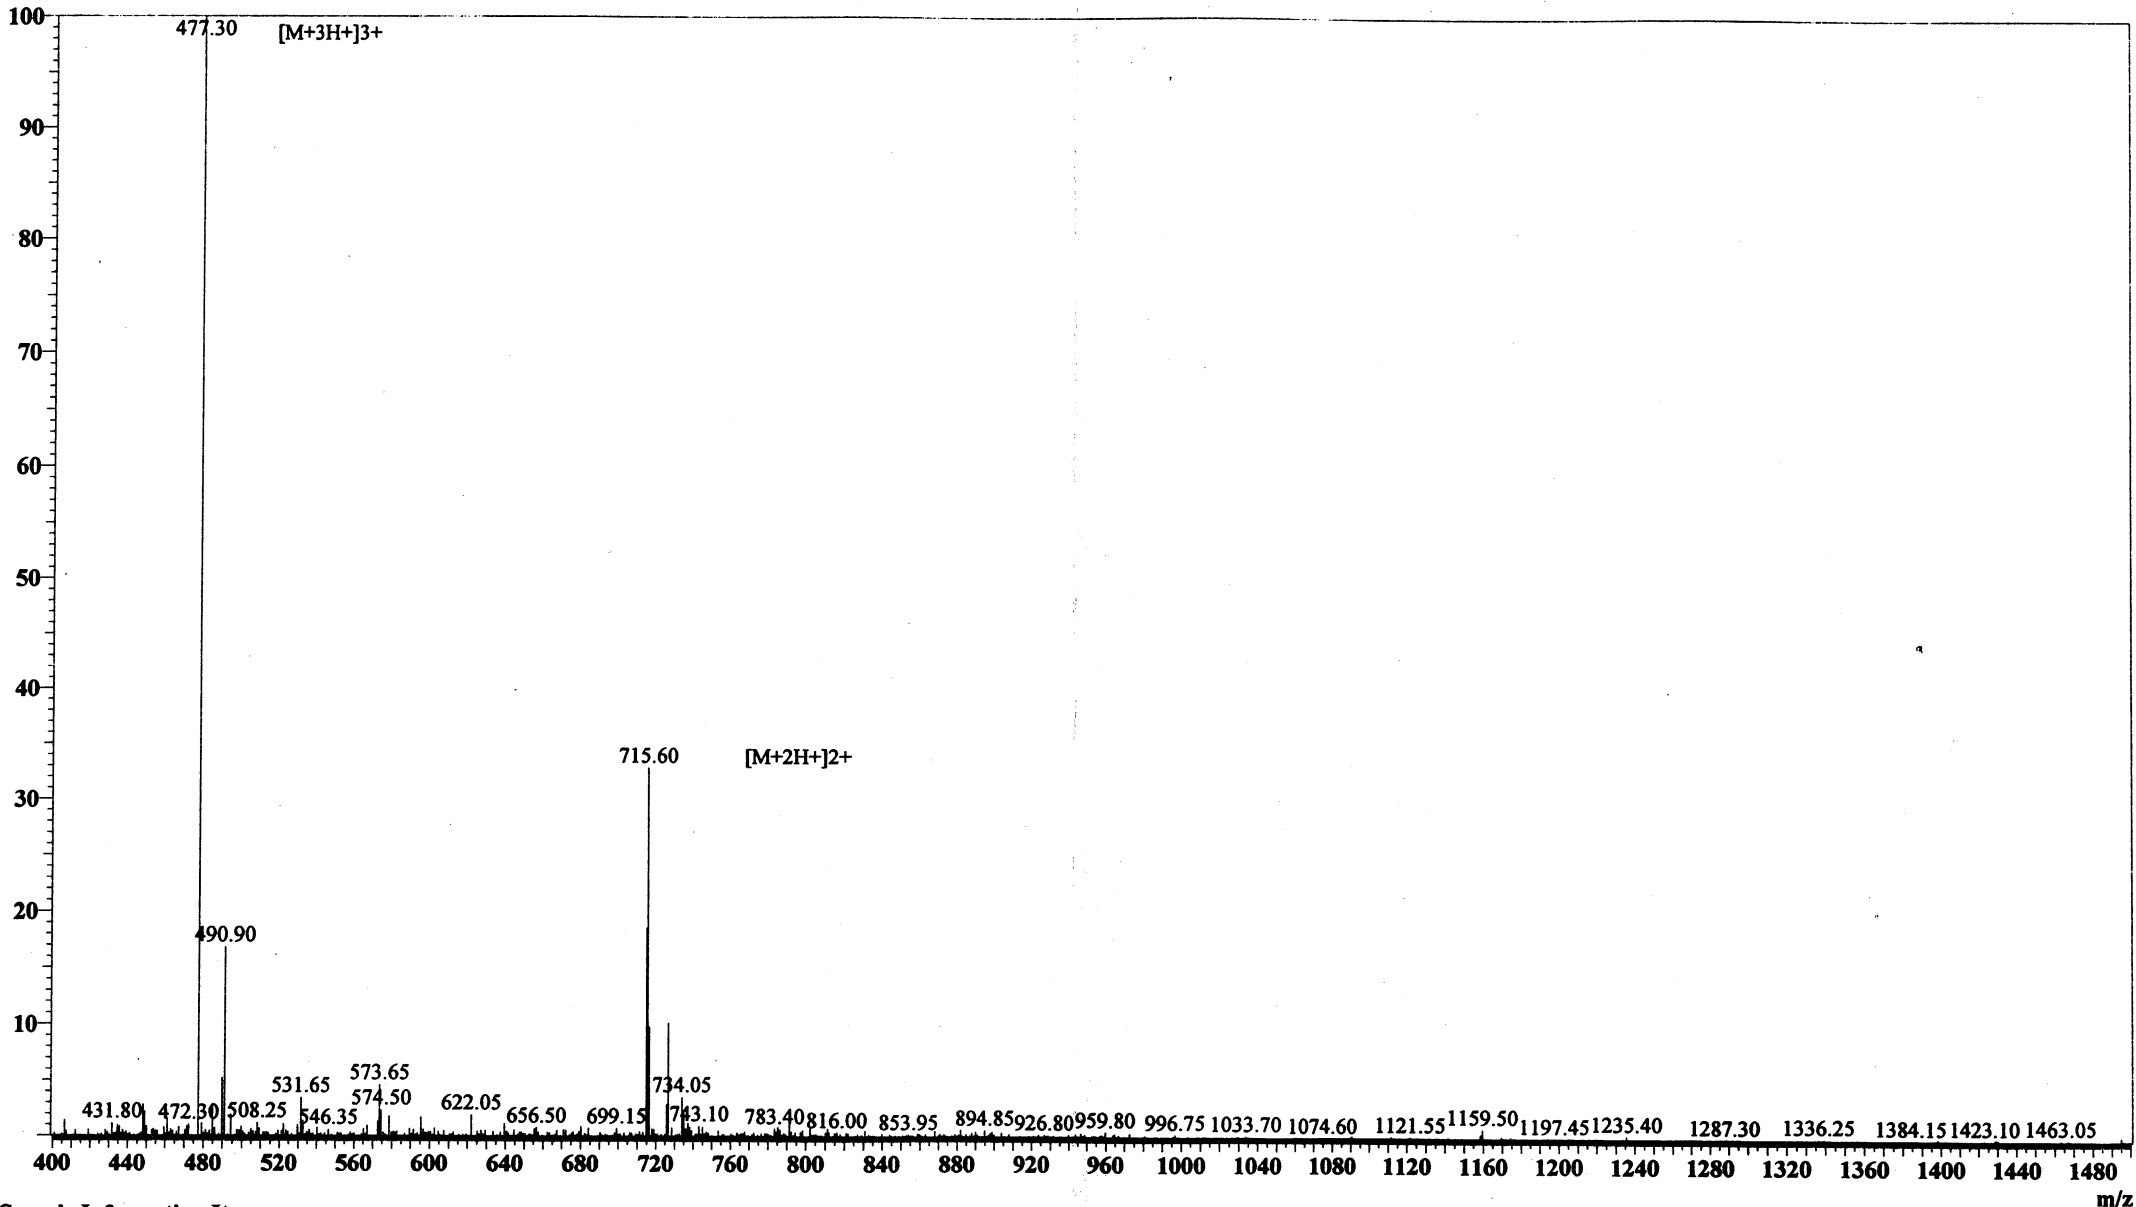

Sample Information Item

Date and Time : 2005-1-15 16:39:11
User : xie
Sample : RP13686(MF-12-NH2)-1
Inj. Volume : 1.000
MW : 1428.709

Cat. No.: RP13686
Lot No.: PJ01225504

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN