


Sample Name : Melittin
 Cat No. :RP10290

Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>
 Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

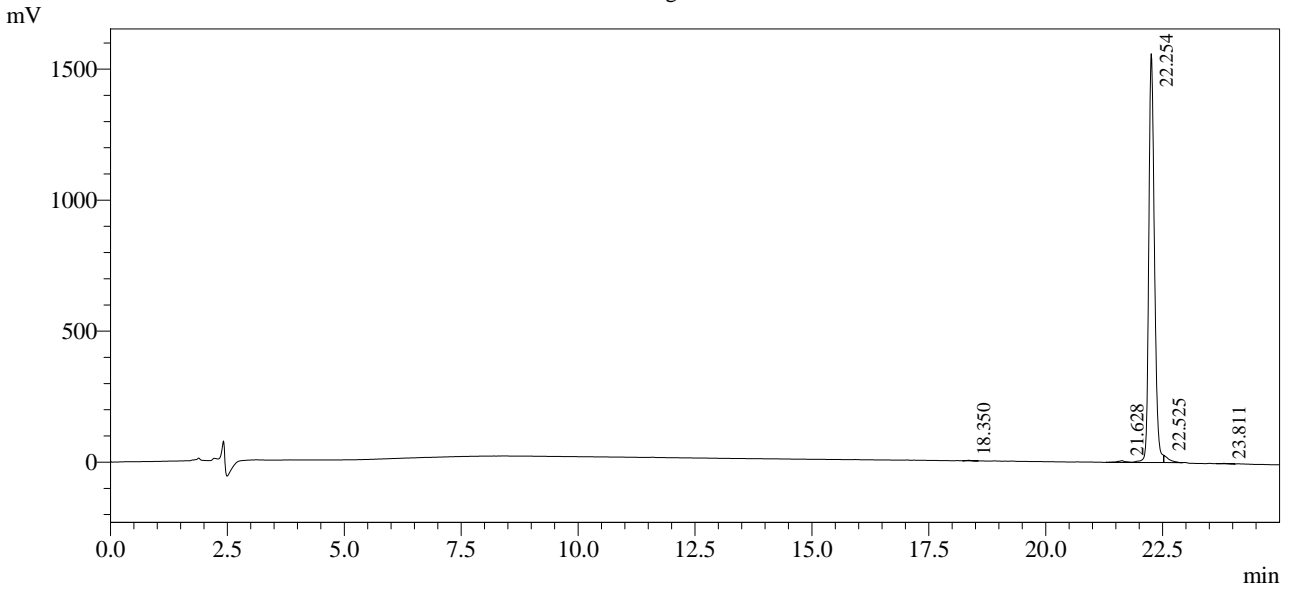

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	18.350	13217	1900	0.098
2	21.628	78442	6673	0.583
3	22.254	13146019	1560426	97.727
4	22.525	200466	28027	1.490
5	23.811	13580	1561	0.101
Total		13451724	1598587	100.000