


Sample Name : PACAP (6-38), human, ovine, rat
 Cat. No. : RP10338
 Lot. No. : 83177002111309ZW

Pump A : 0.065% trifluoroacetic in 100% water (v/v)
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile (v/v)
 Total Flow : 1 ml / min
 Wavelength : 220 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
31.00	Pumps	Pump B Conc.	95	
31.01	Pumps	Pump B Conc.	5	
40.00	Pumps	Pump B Conc.	5	
40.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

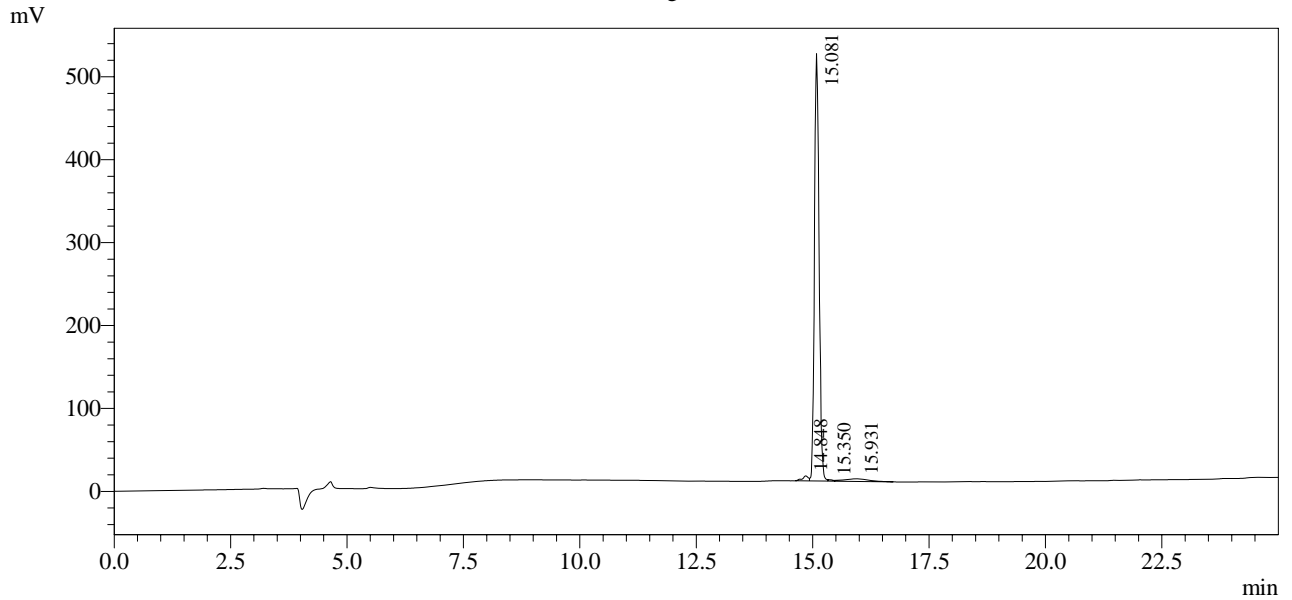

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	14.848	53095	5968	1.413
2	15.081	3577536	515320	95.197
3	15.350	12873	1864	0.343
4	15.931	114523	3122	3.047
Total		3758027	526274	100.000