

Sample Name : Oxytocin
 Cat No. : RP10407


Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

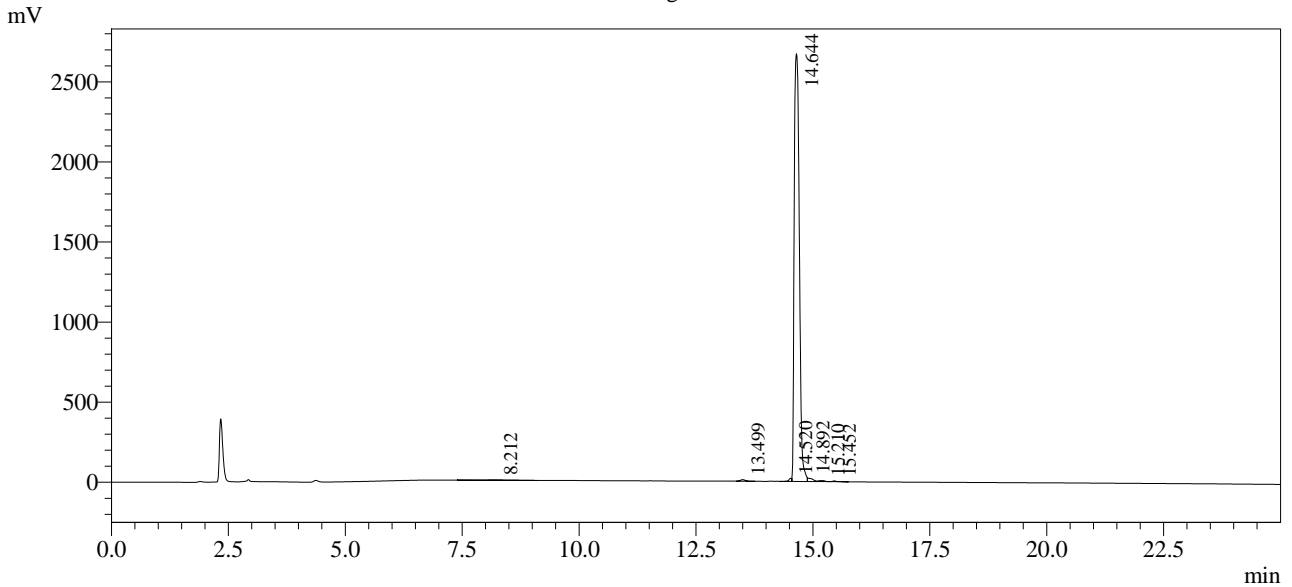

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	8.212	73172	1330	0.352
2	13.499	76073	9637	0.366
3	14.520	91247	19700	0.439
4	14.644	20310601	2670944	97.694
5	14.892	185307	21352	0.891
6	15.210	24397	3832	0.117
7	15.452	29327	4678	0.141
Total		20790124	2731472	100.000