

Sample Name : Oxytocin  
 Cat. No. :RP10407  
 Lot. No. :CC01905

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow:1 ml/min  
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

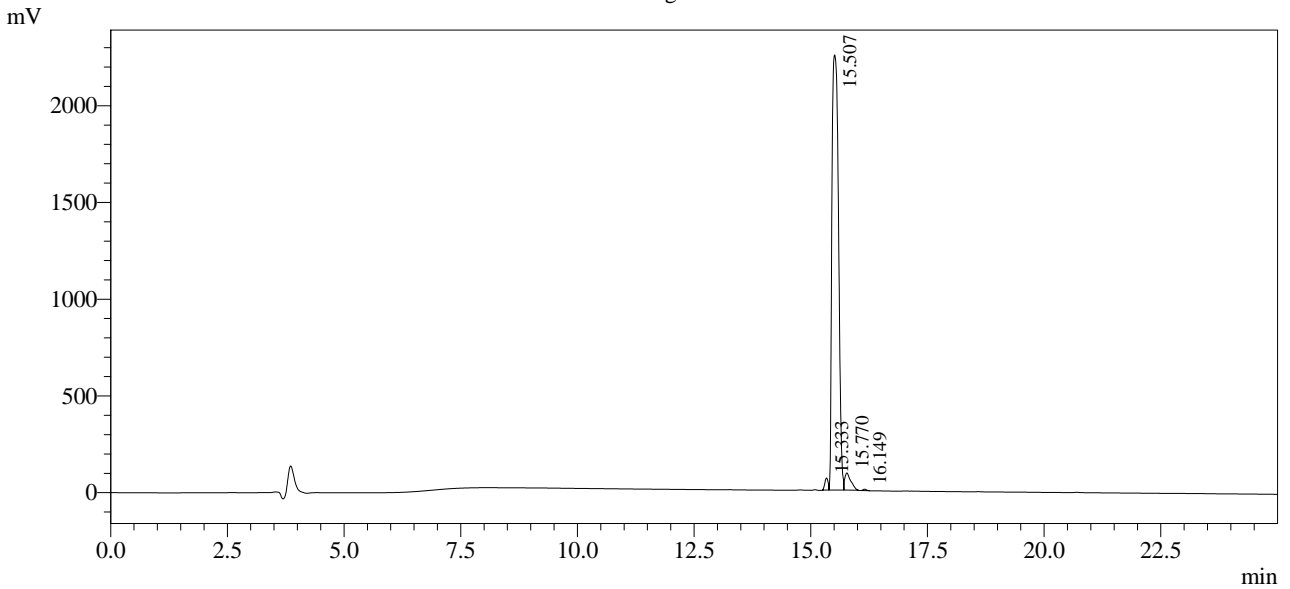

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.333	312942	62112	1.352
2	15.507	22009113	2249505	95.088
3	15.770	790130	88577	3.414
4	16.149	33776	6875	0.146
Total		23145962	2407069	100.000