


Summary:

Structure : PyY-11
 Column : 4.6×250mm, Kromasil
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 : A B
 : 0.01min 16% 84%
 : 25min 32% 68%
 : 25.1min 100% 0%
 : 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

Cat. No.: RP10440
 Lot No.: PJ00621504

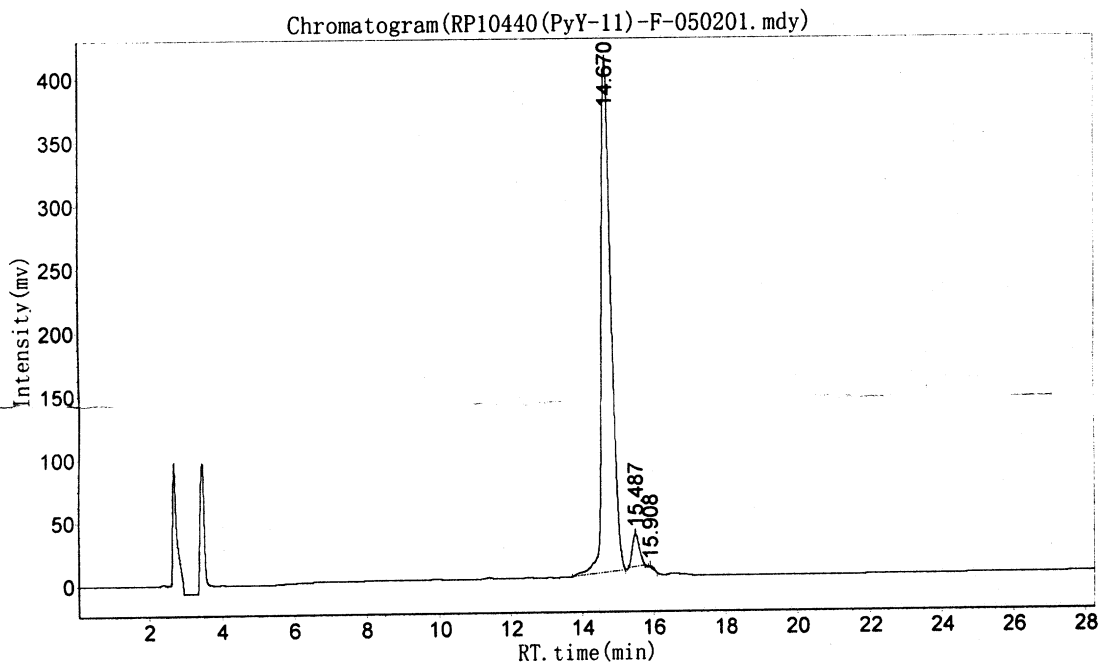

RESULTS

Peak No.	Peak ID	Ret Time	Height	Area	Conc
1		14.670	404792.688	7586048.500	95.3835
2		15.487	25682.525	350316.313	4.4047
3		15.908	1694.082	16841.457	0.2118
TOTAL			432169.294	7953206.270	100.0000