

Sample Name : Neurotensin, guinea pig
 Cat. No. : RP10444
 Lot. No. : CC01910

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

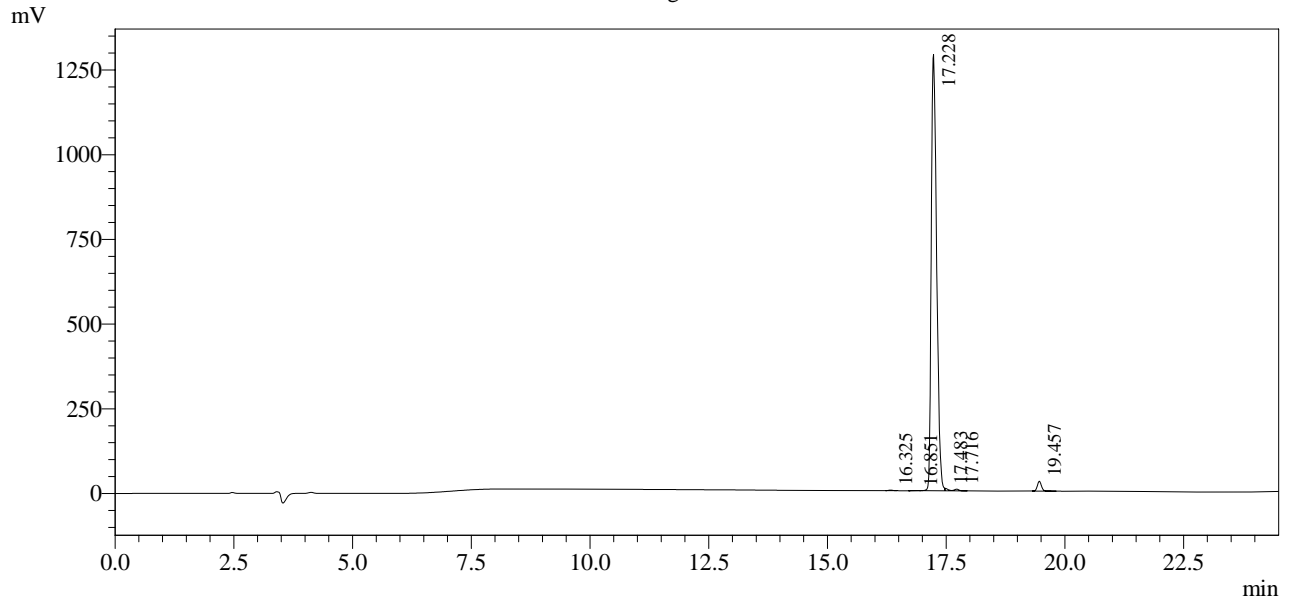

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	16.325	9760	1663	0.094
2	16.851	1579	215	0.015
3	17.228	10134797	1287905	97.567
4	17.483	31136	7362	0.300
5	17.716	35860	5209	0.345
6	19.457	174355	28972	1.679
Total		10387488	1331326	100.000