

Sample Name : DYKDDDDK Peptide
 Cat. No. : RP10586
 Lot. No. : CB08907

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
45.00	Pumps	Pump B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

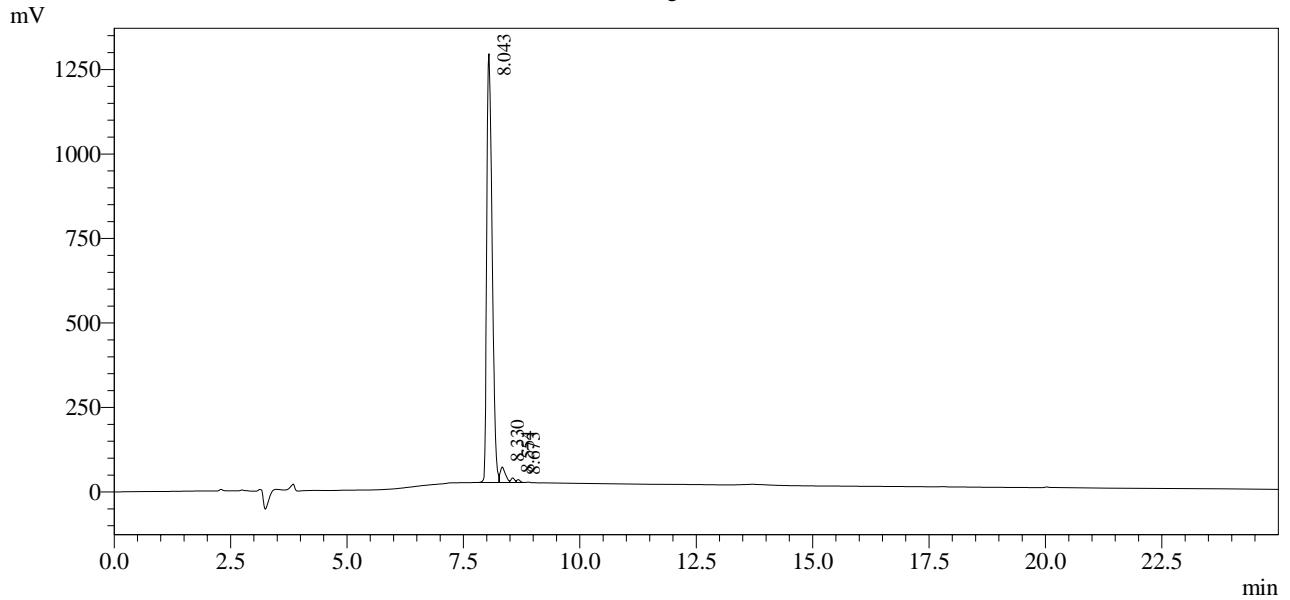

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	8.043	10326458	1268816	95.669
2	8.330	351488	45857	3.256
3	8.554	75700	13497	0.701
4	8.673	40269	8338	0.373
Total		10793915	1336508	100.000