

Sample Name : Mas7  
 Cat. No. : RP10602  
 Lot. No. : CA07907

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow : 1 ml / min  
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : AlltimaTM C18 4.6 x 250 mm

Chromatogram

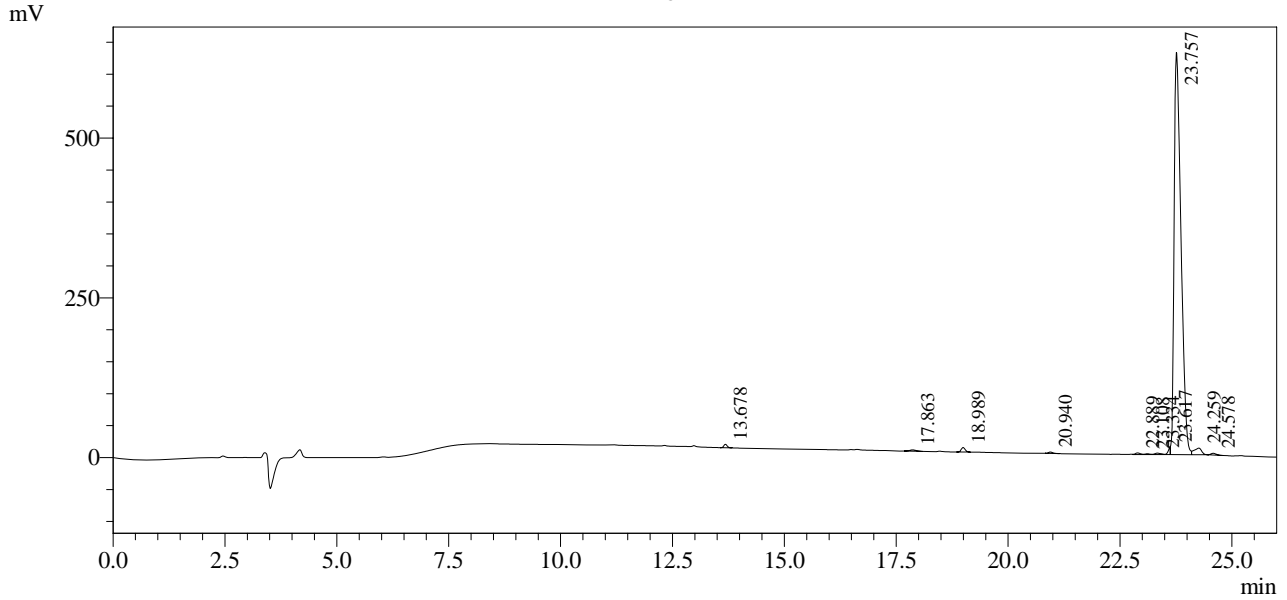

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	13.678	28056	5374	0.396
2	17.863	19453	2003	0.275
3	18.989	43673	7111	0.616
4	20.940	15538	2228	0.219
5	22.889	19535	2470	0.276
6	23.108	9484	1243	0.134
7	23.334	21855	2250	0.308
8	23.617	39190	11817	0.553
9	23.757	6746461	629416	95.219
10	24.259	119724	10334	1.690
11	24.578	22263	2645	0.314
Total		7085231	676892	100.000