


Sample Description:

Structure : RP-10774
 Column : 4.6×250mm, ODS-BP-2
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 : 0.01min A B
 : 25min 35% 65%
 : 25.1min 50% 50%
 : 30min 100% 0%
 STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

Cat. No.: RP10774

Lot No.: PY00226507

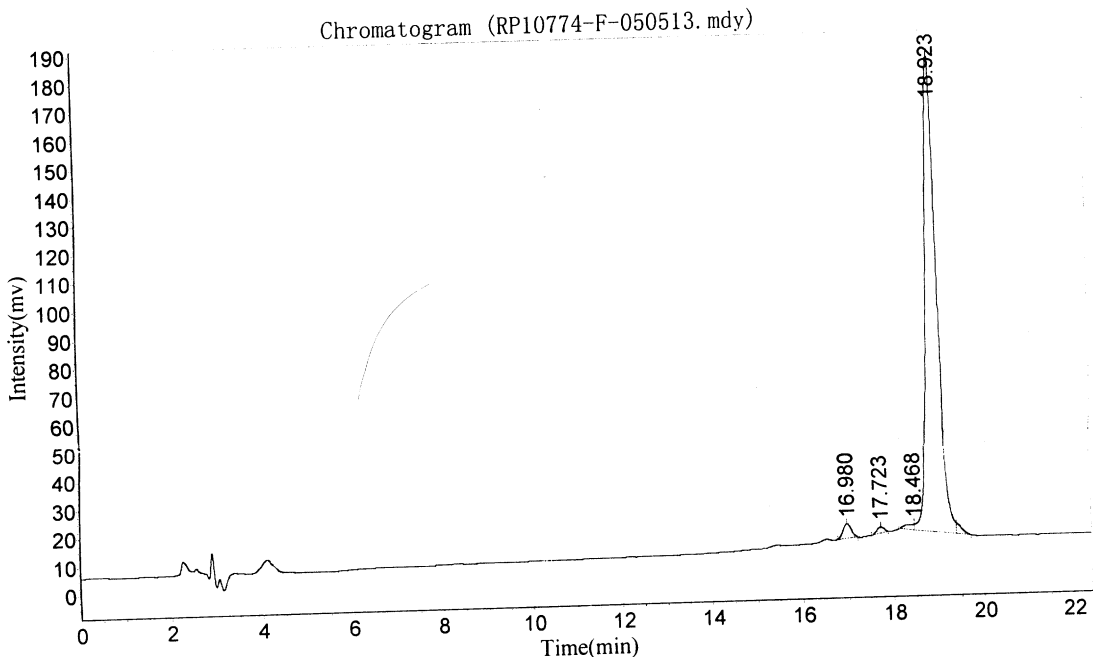

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		16.980	5154.993	65282.309	2.0630
2		17.723	2140.536	24340.285	0.7692
3		18.468	2073.873	27458.314	0.8677
4		18.923	168602.141	3017810.000	95.3668
5		18.923	2918.782	29534.742	0.9333
Total			180890.324	3164425.650	100.0000