

Sample Name : GastricInhibitoryPeptide(GIP),human
 Cat. No. : RP10795

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

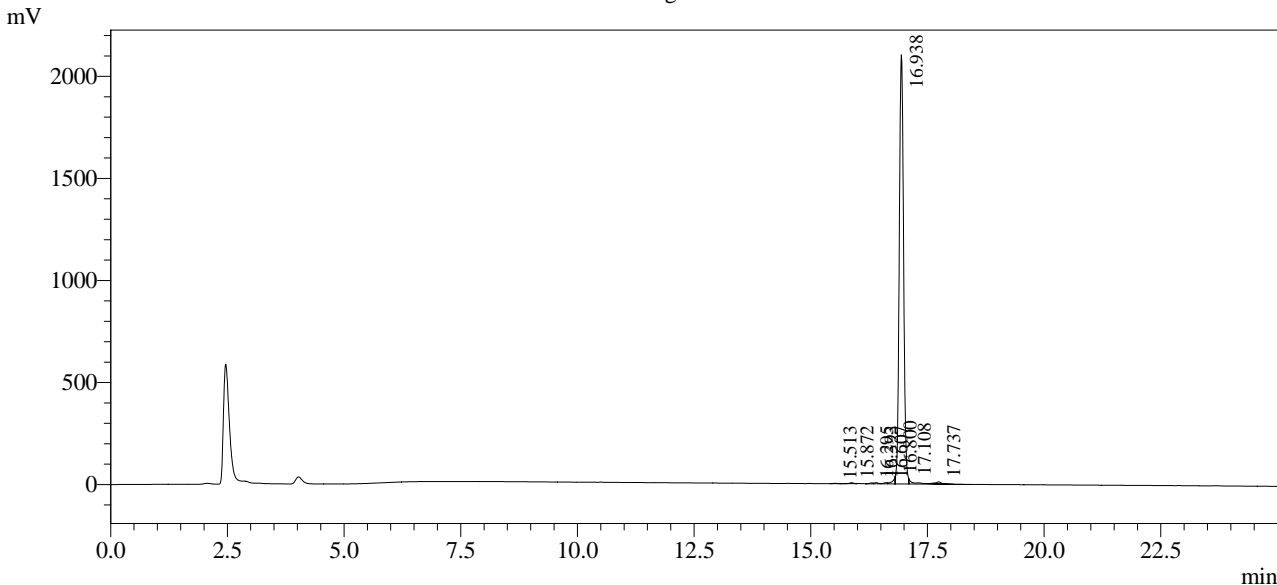

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.513	10512	2043	0.075
2	15.872	31224	5036	0.222
3	16.295	21034	4063	0.150
4	16.393	32971	5415	0.235
5	16.607	34767	5484	0.247
6	16.800	127385	36662	0.907
7	16.938	13505483	2102542	96.119
8	17.108	195274	18335	1.390
9	17.737	92143	9720	0.656
Total		14050794	2189300	100.000