

Sample Name : Arg-Gly-Asp-Cys
 Cat. No. : RP10860
 Lot. No. : CB01905

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
45.00	Pumps	Pump B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

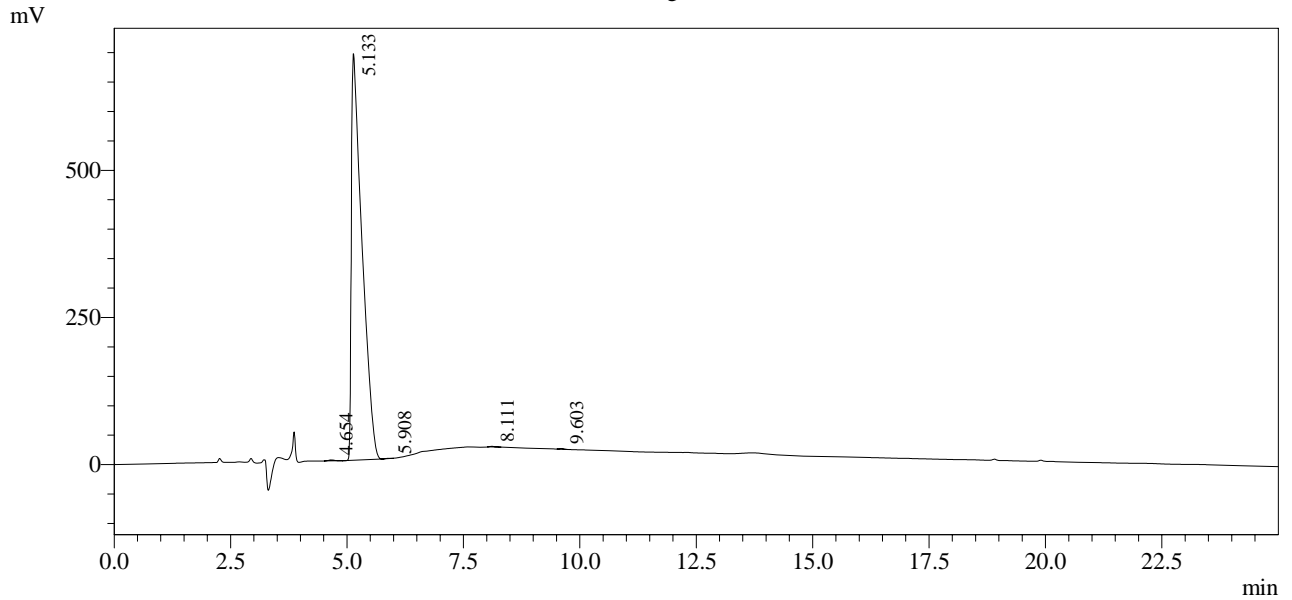

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	4.654	14615	1771	0.132
2	5.133	10997008	690901	99.691
3	5.908	4019	440	0.036
4	8.111	8596	1189	0.078
5	9.603	6910	1203	0.063
Total		11031148	695505	100.000