

Sample Name : Cortistatin 14,human,rat
 Cat. No. : RP10972

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

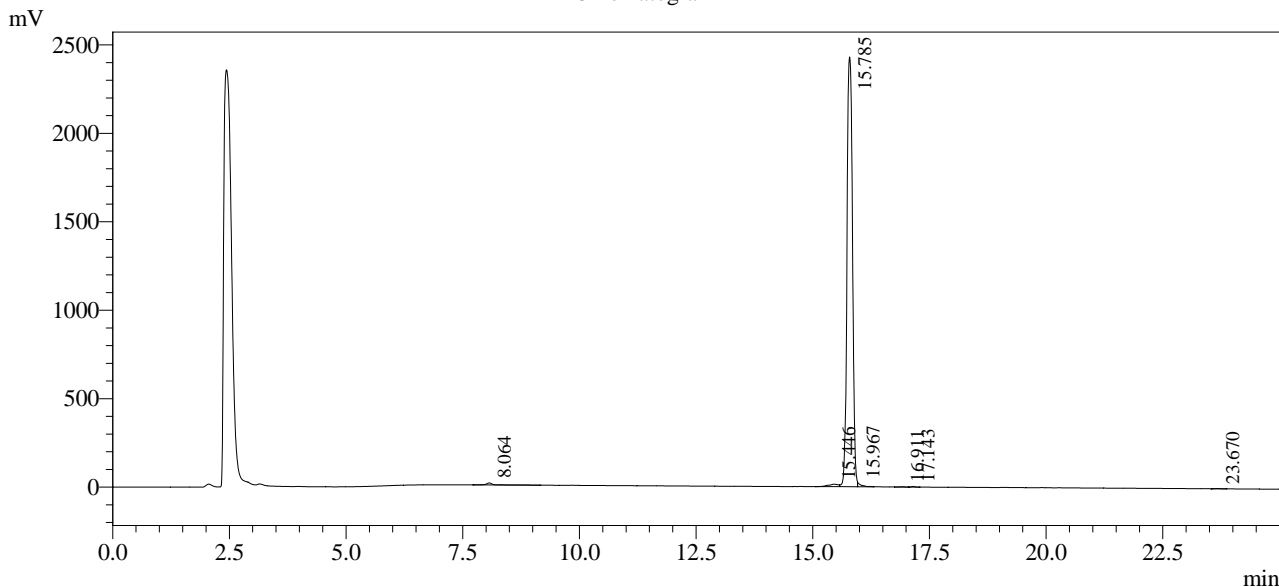

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	8.064	103282	11380	0.508
2	15.446	213592	14106	1.051
3	15.785	19848561	2430178	97.707
4	15.967	105086	18925	0.517
5	16.911	13726	1541	0.068
6	17.143	19260	3778	0.095
7	23.670	10850	1411	0.053
Total		20314357	2481319	100.000