


Sample Description:
 Structure : KS-19
 Column : 4.6×250mm, Kromasil C18-5
 Solvent A : 0.1% trifluoroacetic acid in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic acid in 100% water
 Gradient :
 A B
 0.01min 5% 95%
 25min 25% 75%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0mL/min
 Wavelength : 220nm

Cat. No.: RP11233
 Lot No.: PL00715506

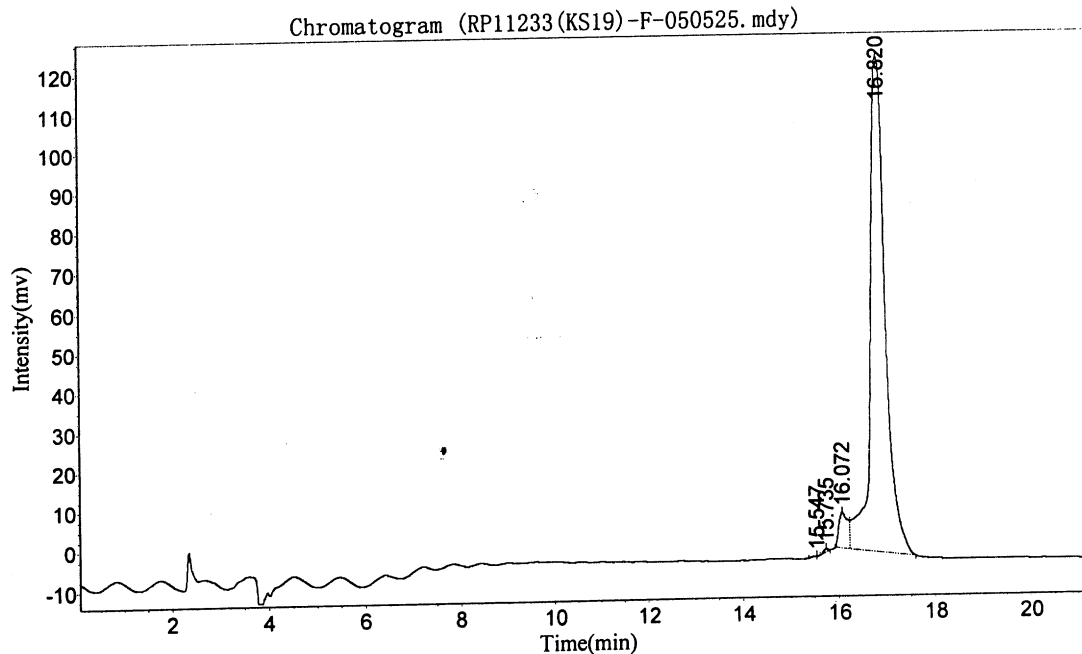

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		15.547	4.215	881.101	0.0307
2		15.735	843.288	5543.849	0.1930
3		16.072	9068.232	117860.453	4.1027
4		16.820	124994.367	2748473.500	95.6737
Total			134910.102	2872758.903	100.0000