

Sample Name : Angiotensin II,human
 Cat. No. : RP11257
 Lot. No. : CD01902

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

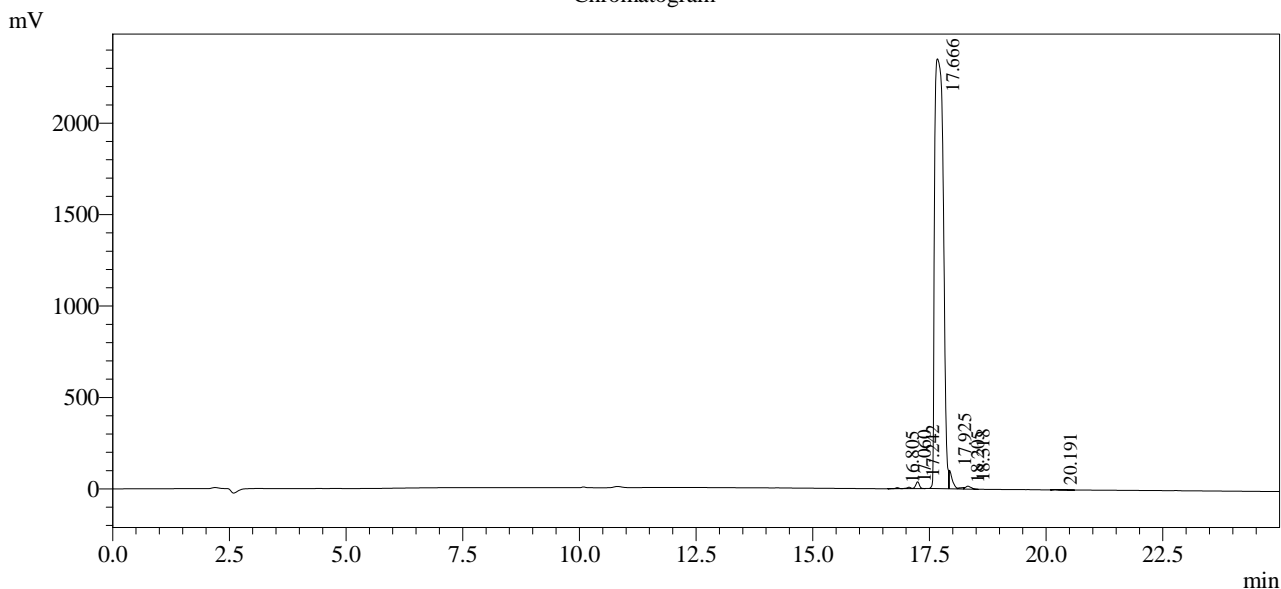

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	16.805	31424	5995	0.100
2	17.060	46413	7857	0.148
3	17.242	201910	36964	0.645
4	17.666	30356828	2350334	96.993
5	17.925	472472	101151	1.510
6	18.205	51097	7262	0.163
7	18.318	126643	16023	0.405
8	20.191	11091	1688	0.035
Total		31297878	2527273	100.000