


Sample Description:
 Structure : SG-10
 Column : 4.6×250mm, VYDAC-C18
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 : A B
 0.01min 18% 82%
 25min 60% 40%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

Cat. No.: RP11299
 Lot No.: PJ00125504

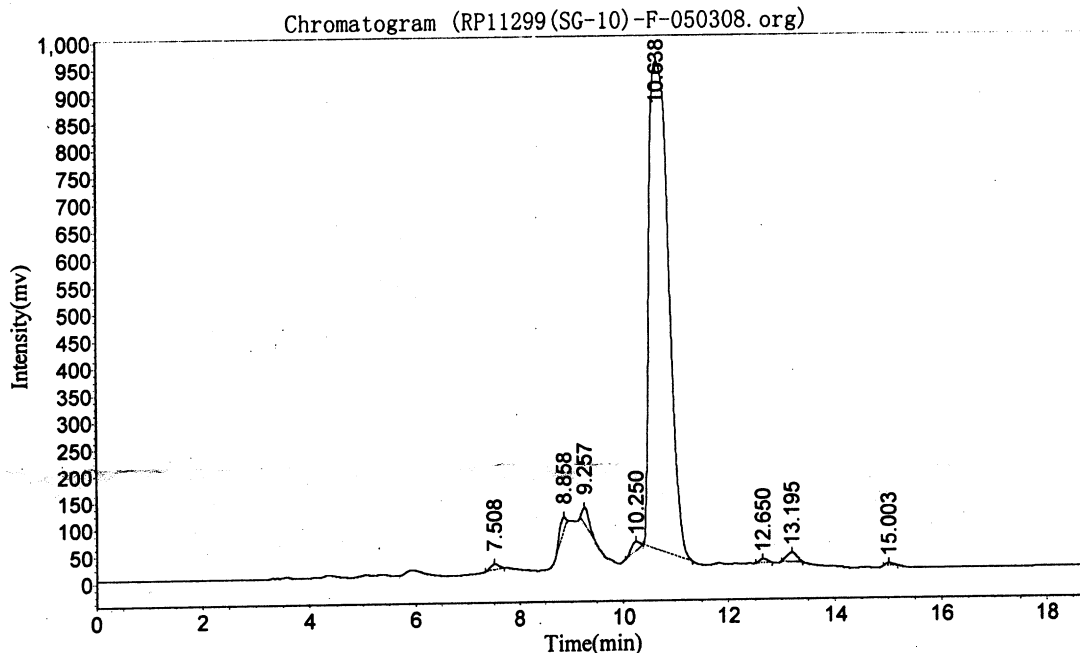

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		7.508	10807.197	120794.531	0.4944
2		8.858	27533.676	244993.547	1.0027
3		9.257	29904.816	288758.375	1.1818
4		10.250	16685.078	192630.344	0.7884
5		10.638	903585.188	23240494.000	95.1147
6		12.650	6910.535	71625.656	0.2931
7		13.195	17331.078	224229.688	0.9177
8		15.003	5526.038	50662.898	0.2073
Total			1018283.606	24434189.039	100.0000