

Sample Name : Dermorphin Analog  
 Cat. No. :RP13522  
 Lot. No. :83177004111309WJ

Pump A : 0.065% trifluoroacetic in 100% water  
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile  
 Total Flow:1 ml/min  
 Wavelength:220 nm


| Time  | Unit       | Command       | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01  | Pumps      | Pump A B.Conc | 5     |         |
| 25.00 | Pumps      | Pump A B.Conc | 65    |         |
| 25.01 | Pumps      | Pump A B.Conc | 95    |         |
| 31.00 | Pumps      | Pump A B.Conc | 95    |         |
| 31.01 | Pumps      | Pump A B.Conc | 5     |         |
| 40.00 | Pumps      | Pump A B.Conc | 5     |         |
| 40.01 | Controller | Stop          |       |         |

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

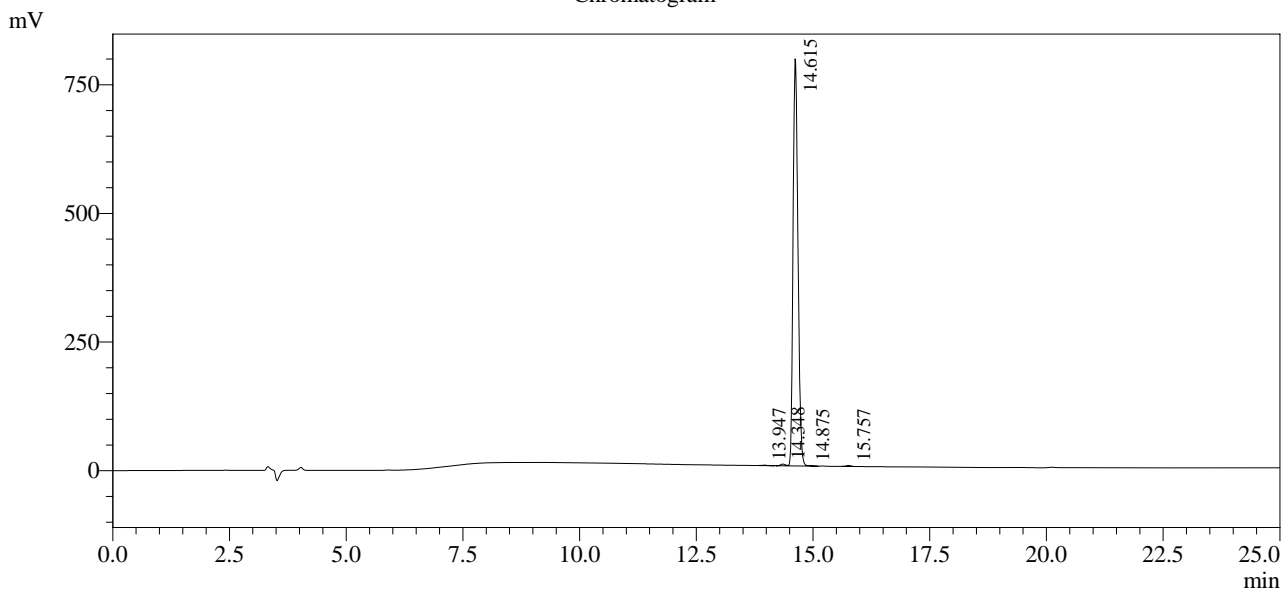

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

| Peak# | Ret. Time | Area    | Height | Area %  |
|-------|-----------|---------|--------|---------|
| 1     | 13.947    | 7082    | 1019   | 0.121   |
| 2     | 14.348    | 23833   | 3258   | 0.408   |
| 3     | 14.615    | 5792539 | 791059 | 99.169  |
| 4     | 14.875    | 5390    | 944    | 0.092   |
| 5     | 15.757    | 12239   | 1791   | 0.210   |
| Total |           | 5841083 | 798072 | 100.000 |