


Sample Name : Ub2
 Cat No. : RP19981

Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>
 Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

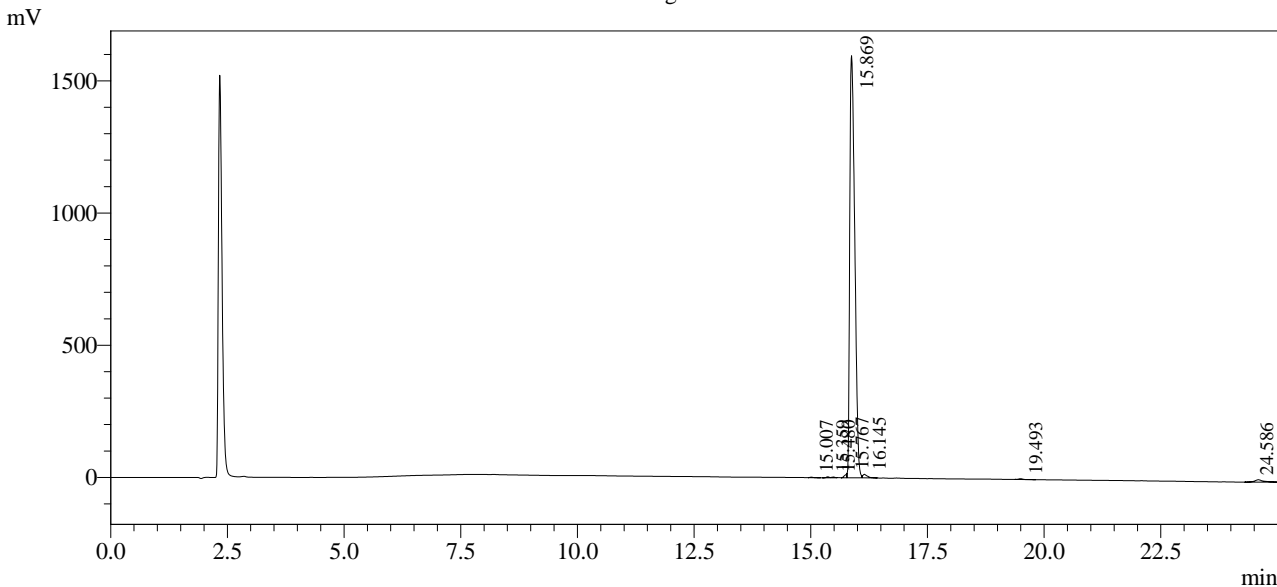

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.007	10087	2018	0.082
2	15.359	16186	3704	0.132
3	15.480	13427	2686	0.109
4	15.767	53601	14494	0.437
5	15.869	11955231	1596365	97.378
6	16.145	88992	13322	0.725
7	19.493	18215	3080	0.148
8	24.586	121445	8878	0.989
Total		12277184	1644548	100.000