

Sample Name : Tetanus toxin (830-843)
 Cat. No. : RP19980


Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

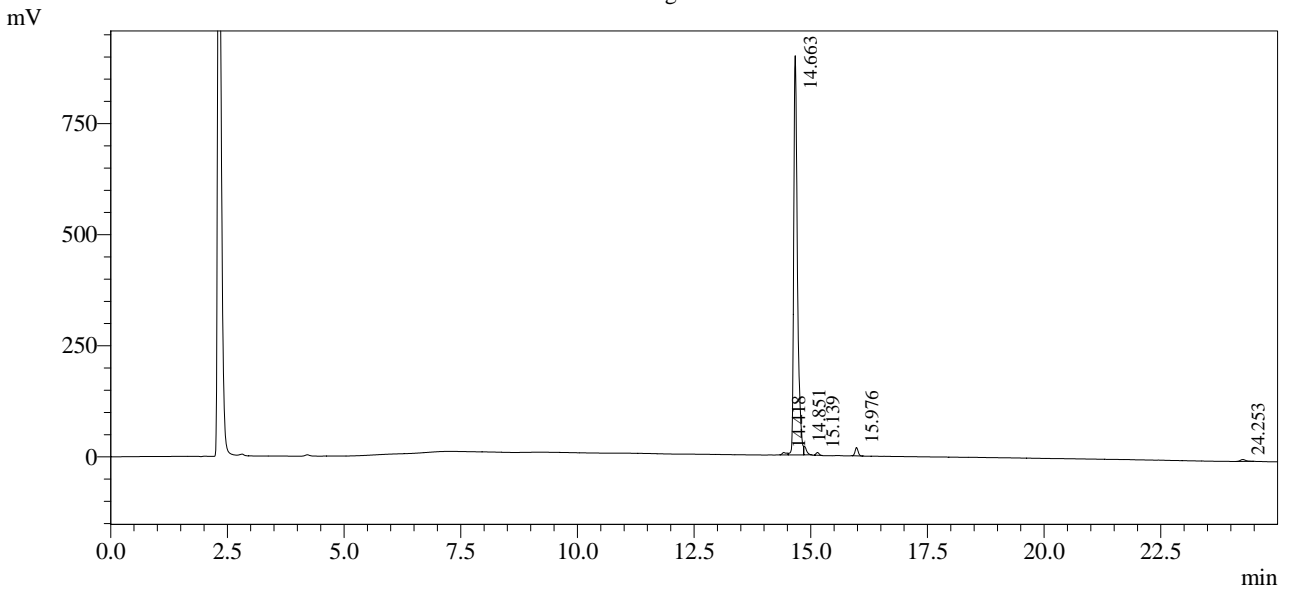

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	14.418	39145	5406	0.745
2	14.663	5000019	898356	95.143
3	14.851	70198	19128	1.336
4	15.139	26967	6056	0.513
5	15.976	85032	18619	1.618
6	24.253	33903	4266	0.645
Total		5255265	951831	100.000