

Sample Name :MOG
 Cat. No. :RP10245
 Lot. No. :CA06910

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:220 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.01	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.01	Pumps	Pump A B.Conc	5	
45.00	Pumps	Pump A B.Conc	5	
45.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

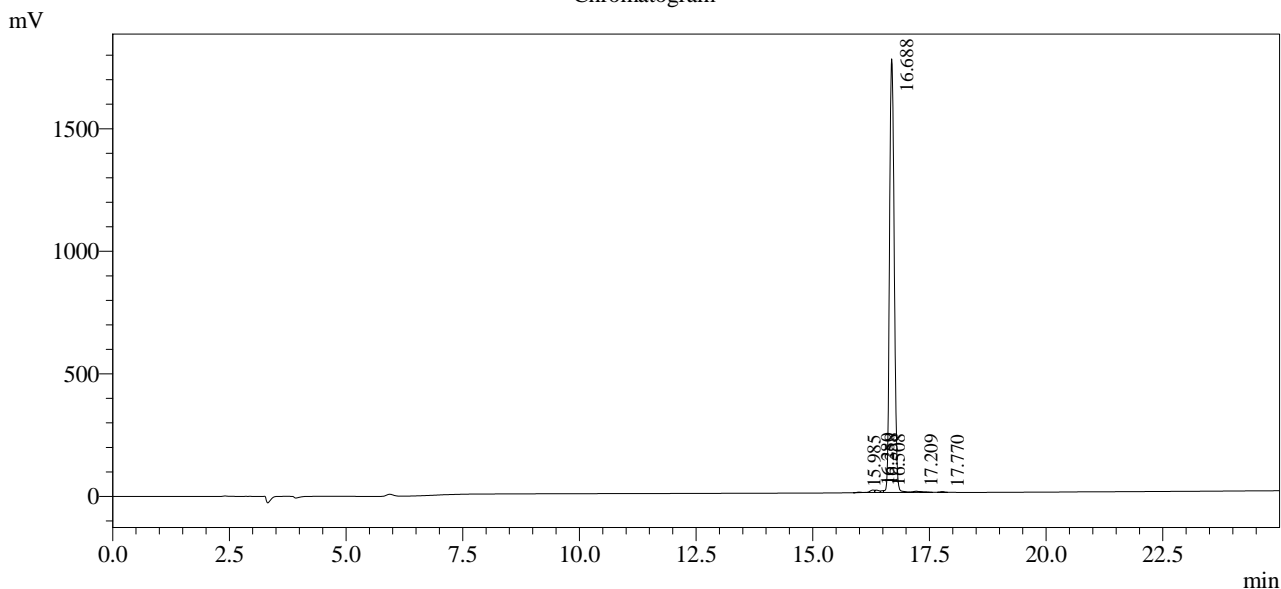

1 Det.A Ch1 / 220nm

Peak Table

Detector A Ch1 220nm

Peak#	Ret. Time	Area	Height	Area %
1	15.985	12503	2024	0.098
2	16.280	63291	9776	0.498
3	16.358	61228	9537	0.482
4	16.508	27800	7422	0.219
5	16.688	12467237	1768929	98.100
6	17.209	64162	4673	0.505
7	17.770	12455	2385	0.098
Total		12708675	1804746	100.000