


Sample Name : Glycoprotein(276-286)
 Cat No. : RP19983

Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>
 Column : SHIMADZU VP-ODS 4.6 x 150 mm

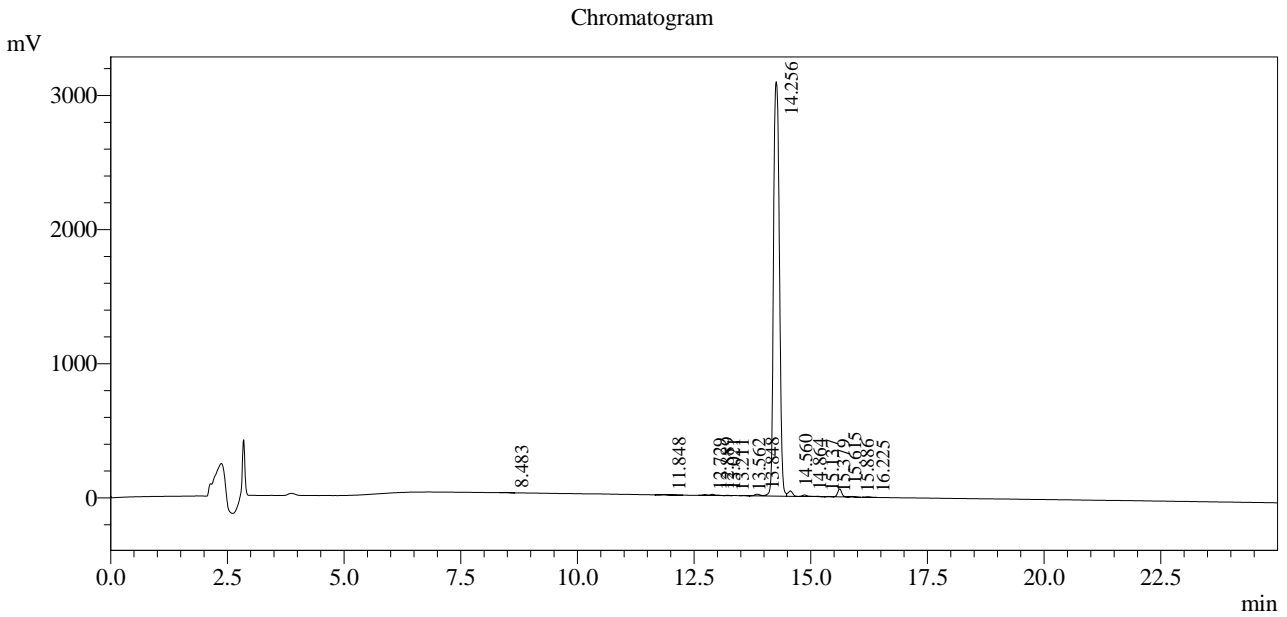

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	8.483	19887	2843	0.071
2	11.848	35826	3665	0.128
3	12.729	38480	5501	0.137
4	12.889	58848	8708	0.210
5	13.021	11397	2445	0.041
6	13.211	10334	2159	0.037
7	13.562	11345	2204	0.041
8	13.848	101848	12422	0.364
9	14.256	26961012	3089719	96.252
10	14.560	268243	39275	0.958
11	14.864	72087	10940	0.257
12	15.137	12583	2465	0.045
13	15.379	11913	2258	0.043
14	15.615	346510	58928	1.237
15	15.886	25373	3975	0.091
16	16.225	25073	3735	0.090
Total		28010759	3251242	100.000