


Sample Name : KLKL5KLK
 Cat. No. : RP20088
 Lot. No. : CA02905

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump B Conc.	5	
25.00	Pumps	Pump B Conc.	65	
25.01	Pumps	Pump B Conc.	95	
35.00	Pumps	Pump B Conc.	95	
35.01	Pumps	Pump B Conc.	5	
45.00	Pumps	Pump B Conc.	5	
45.01	Controller	Stop		

<<Column Performance>>
 <Detector A>
 Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

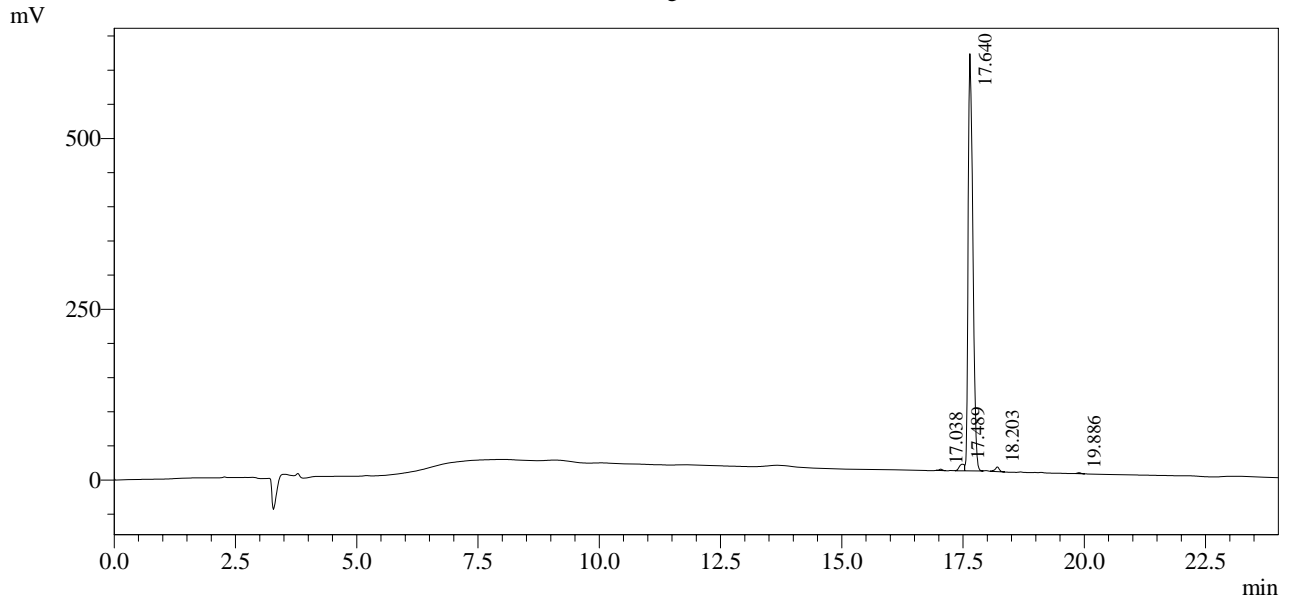

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	17.038	8355	1892	0.196
2	17.489	71515	9785	1.682
3	17.640	4126214	610711	97.026
4	18.203	39962	6879	0.940
5	19.886	6635	1378	0.156
Total		4252681	630644	100.000