

Sample Name : LAH4
 Cat No. : RP20096


Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

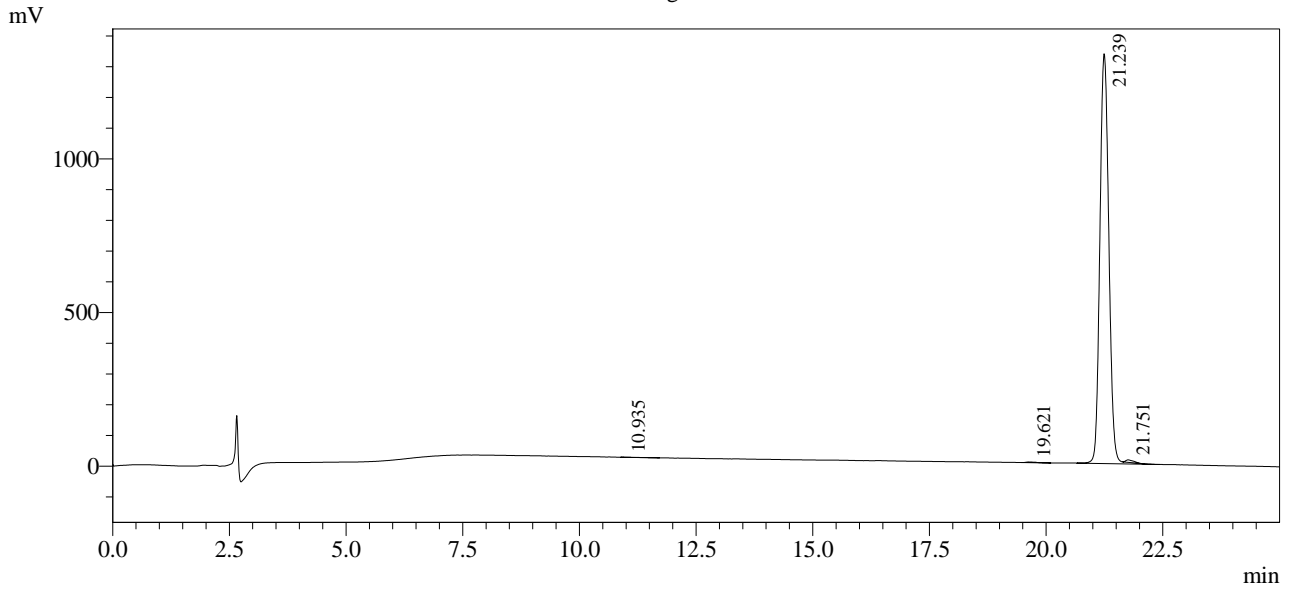

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	10.935	11665	475	0.065
2	19.621	33618	2345	0.187
3	21.239	17864628	1333755	99.207
4	21.751	97498	8074	0.541
Total		18007409	1344650	100.000