

Sample Name : Mca-SE...K(Dnp)-RR-NH2
 Cat. No. :RP20114
 Lot. No. :CR01906

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm


| Time | Unit | Command | Value | Comment |
|-------|------------|---------------|-------|---------|
| 0.01 | Pumps | Pump A B.Conc | 5 | |
| 25.00 | Pumps | Pump A B.Conc | 65 | |
| 25.10 | Pumps | Pump A B.Conc | 95 | |
| 33.00 | Pumps | Pump A B.Conc | 95 | |
| 33.10 | Pumps | Pump A B.Conc | 5 | |
| 43.00 | Pumps | Pump A B.Conc | 5 | |
| 43.10 | Controller | Stop | | |

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

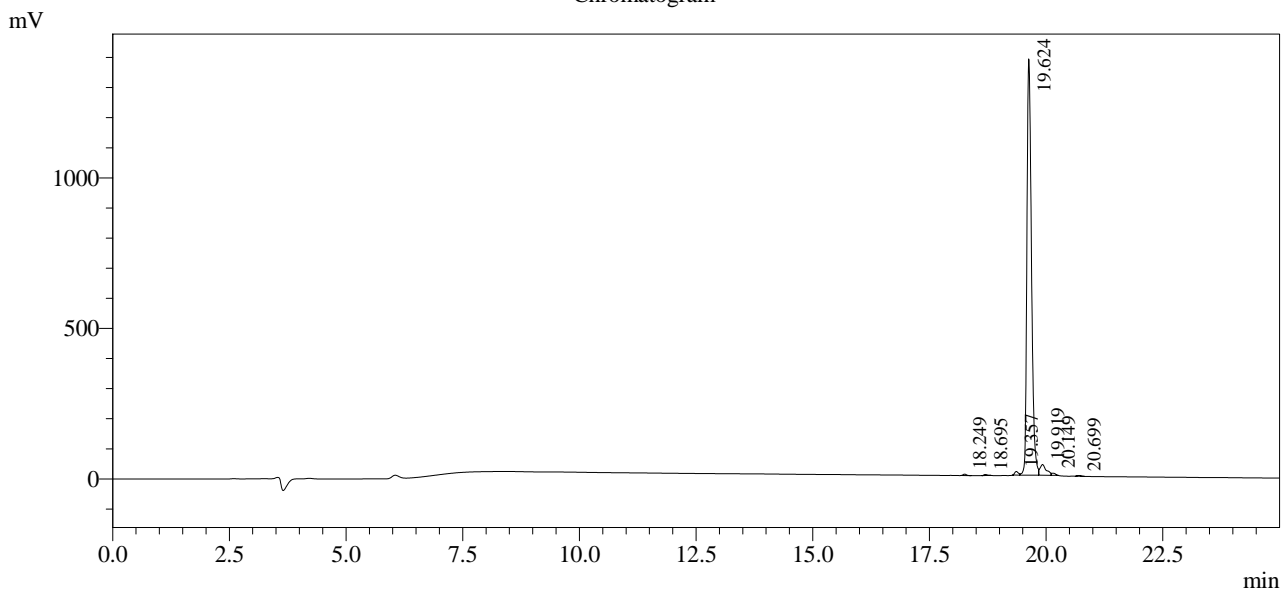

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

| Peak# | Ret. Time | Area | Height | Area % |
|-------|-----------|---------|---------|---------|
| 1 | 18.249 | 24061 | 4638 | 0.243 |
| 2 | 18.695 | 16011 | 3385 | 0.162 |
| 3 | 19.357 | 67485 | 12010 | 0.682 |
| 4 | 19.624 | 9402559 | 1382970 | 95.008 |
| 5 | 19.919 | 335172 | 35782 | 3.387 |
| 6 | 20.149 | 39442 | 7114 | 0.399 |
| 7 | 20.699 | 11837 | 2345 | 0.120 |
| Total | | 9896567 | 1448244 | 100.000 |