

Sample Name : KLKLLLLLKLK-NH2
 Cat No. : RP20089


Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

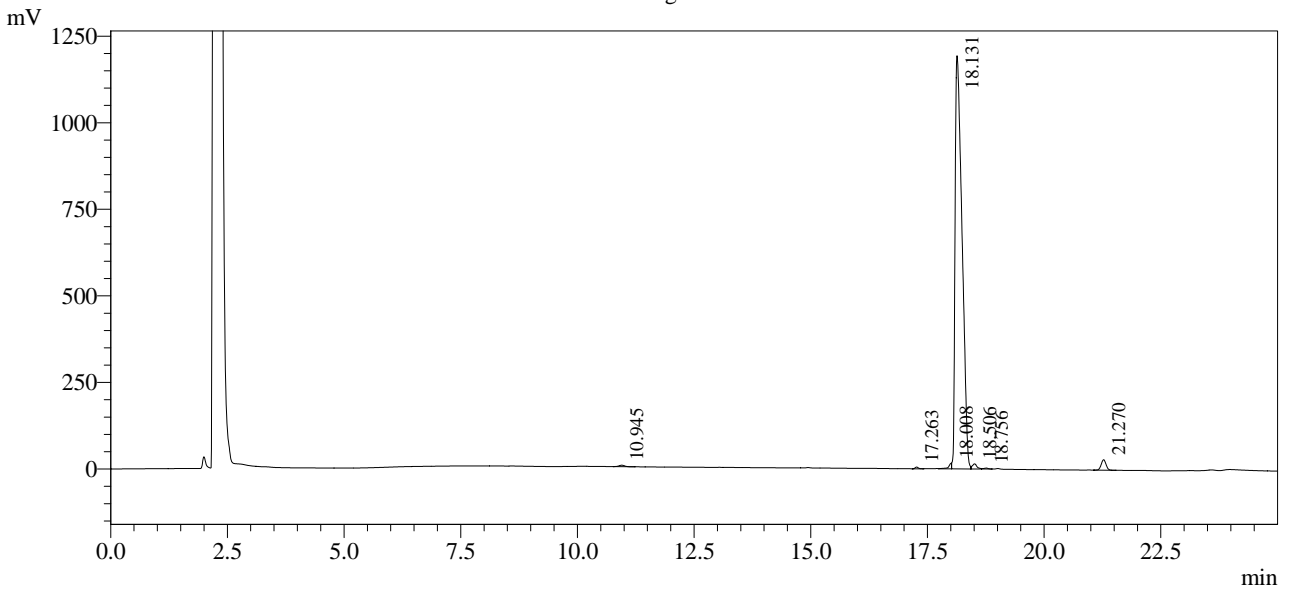

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	10.945	35024	4162	0.274
2	17.263	23706	5088	0.185
3	18.008	76972	16929	0.601
4	18.131	12330332	1193313	96.288
5	18.506	101349	14886	0.791
6	18.756	18324	2650	0.143
7	21.270	219922	30190	1.717
Total		12805627	1267218	100.000