


Sample Description:

Structure : RS-4
 Column : 4.6×250mm, Sinochrom ODS-BP-5
 Solvent A : 0.1% trifluoroacetic in 100% acetonitrile
 Solvent B : 0.1% trifluoroacetic in 100% water
 Gradient :
 A B
 0.01min 2% 98%
 25min 15% 85%
 25.1min 100% 0%
 30min STOP
 Flow rate : 1.0 mL/min
 Wavelength : 220nm

RP10861

PY00105509

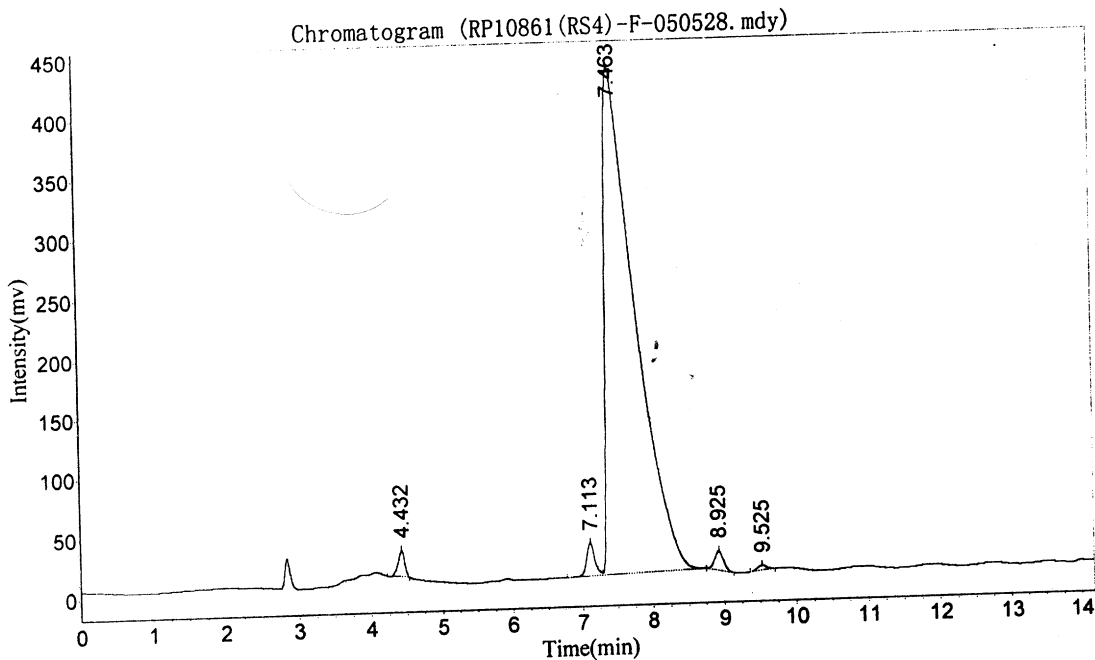

Results

Peak No.	Peak ID	Ret Time	Height	Area	Conc.
1		4.432	21980.414	136773.000	1.0479
2		7.113	28021.639	225584.203	1.7283
3		7.463	426467.656	12510911.000	95.8522
4		8.925	16021.080	140508.500	1.0765
5		9.525	4284.656	38513.996	0.2951
Total			496775.445	13052290.699	100.0000