


Sample Name : CEF20
 Cat No. : RP11781

Pump A : 0.065% trifluoroacetic in 100% water
 Pump A : 0.05% trifluoroacetic in 100% acetonitrile
 TotalFlow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
30.00	Pumps	Pump A B.Conc	100	
42.00	Pumps	Pump A B.Conc	100	
43.00	Pumps	Pump A B.Conc	5	
49.00	Pumps	Pump A B.Conc	5	
50.00	Controller	Stop		

<Detector A>
 Column : SHIMADZU VP-ODS 4.6 x 150 mm

Chromatogram

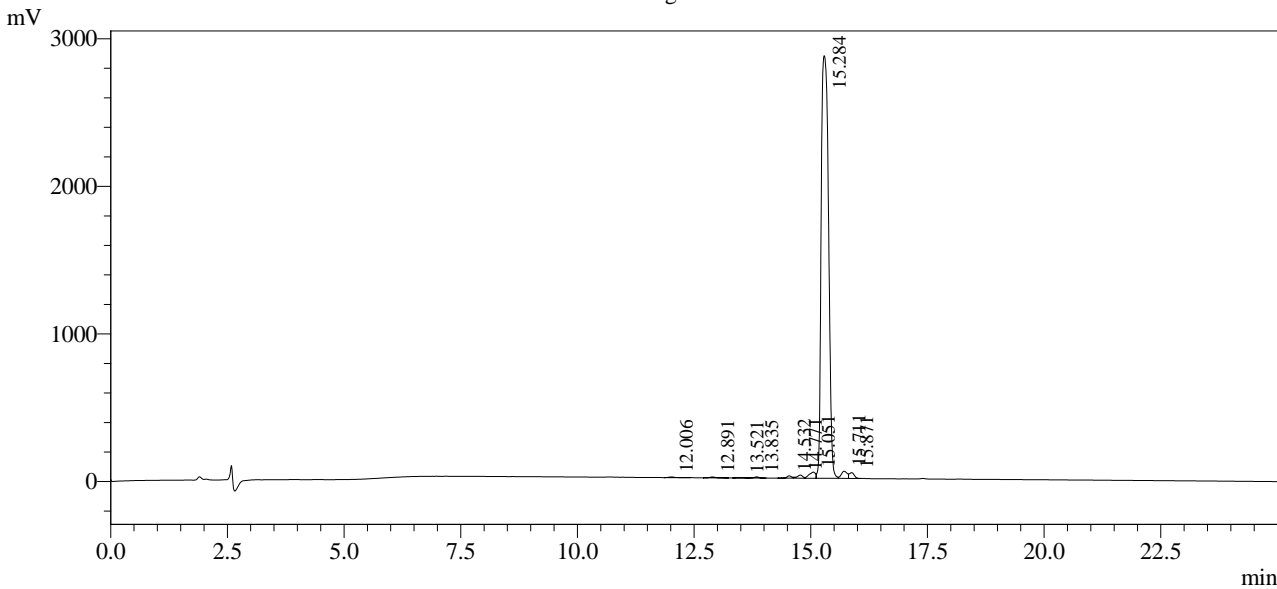

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	12.006	42063	4606	0.128
2	12.891	53399	6353	0.163
3	13.521	12957	1219	0.039
4	13.835	54465	7852	0.166
5	14.532	107846	15529	0.329
6	14.771	176969	21361	0.539
7	15.051	394055	41490	1.201
8	15.284	31263012	2863208	95.287
9	15.711	426274	48098	1.299
10	15.871	278181	38676	0.848
Total		32809221	3048391	100.000