

Sample Name : EGFR(988-993)(Phospho-Tyr5)
 Cat. No. :RP20108


Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow:1 ml/min
 Wavelength:214 nm

Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
33.00	Pumps	Pump A B.Conc	95	
33.10	Pumps	Pump A B.Conc	5	
43.00	Pumps	Pump A B.Conc	5	
43.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : SHIMADZU VP-ODS 4.6 x 150 mm

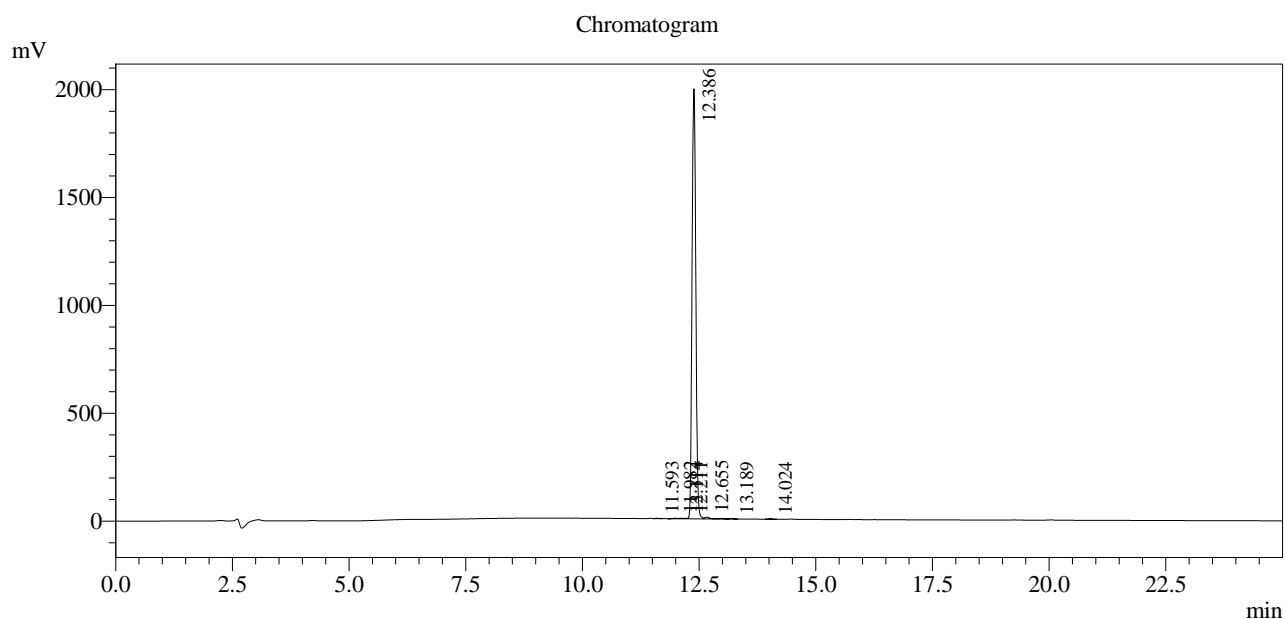

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	11.593	6868	1678	0.060
2	11.982	13505	2207	0.119
3	12.114	14820	2420	0.131
4	12.211	8668	2094	0.076
5	12.386	11232262	1993280	98.919
6	12.655	58460	7667	0.515
7	13.189	9676	1981	0.085
8	14.024	10751	2275	0.095
Total		11355010	2013603	100.000