


Positive MS Spectrum

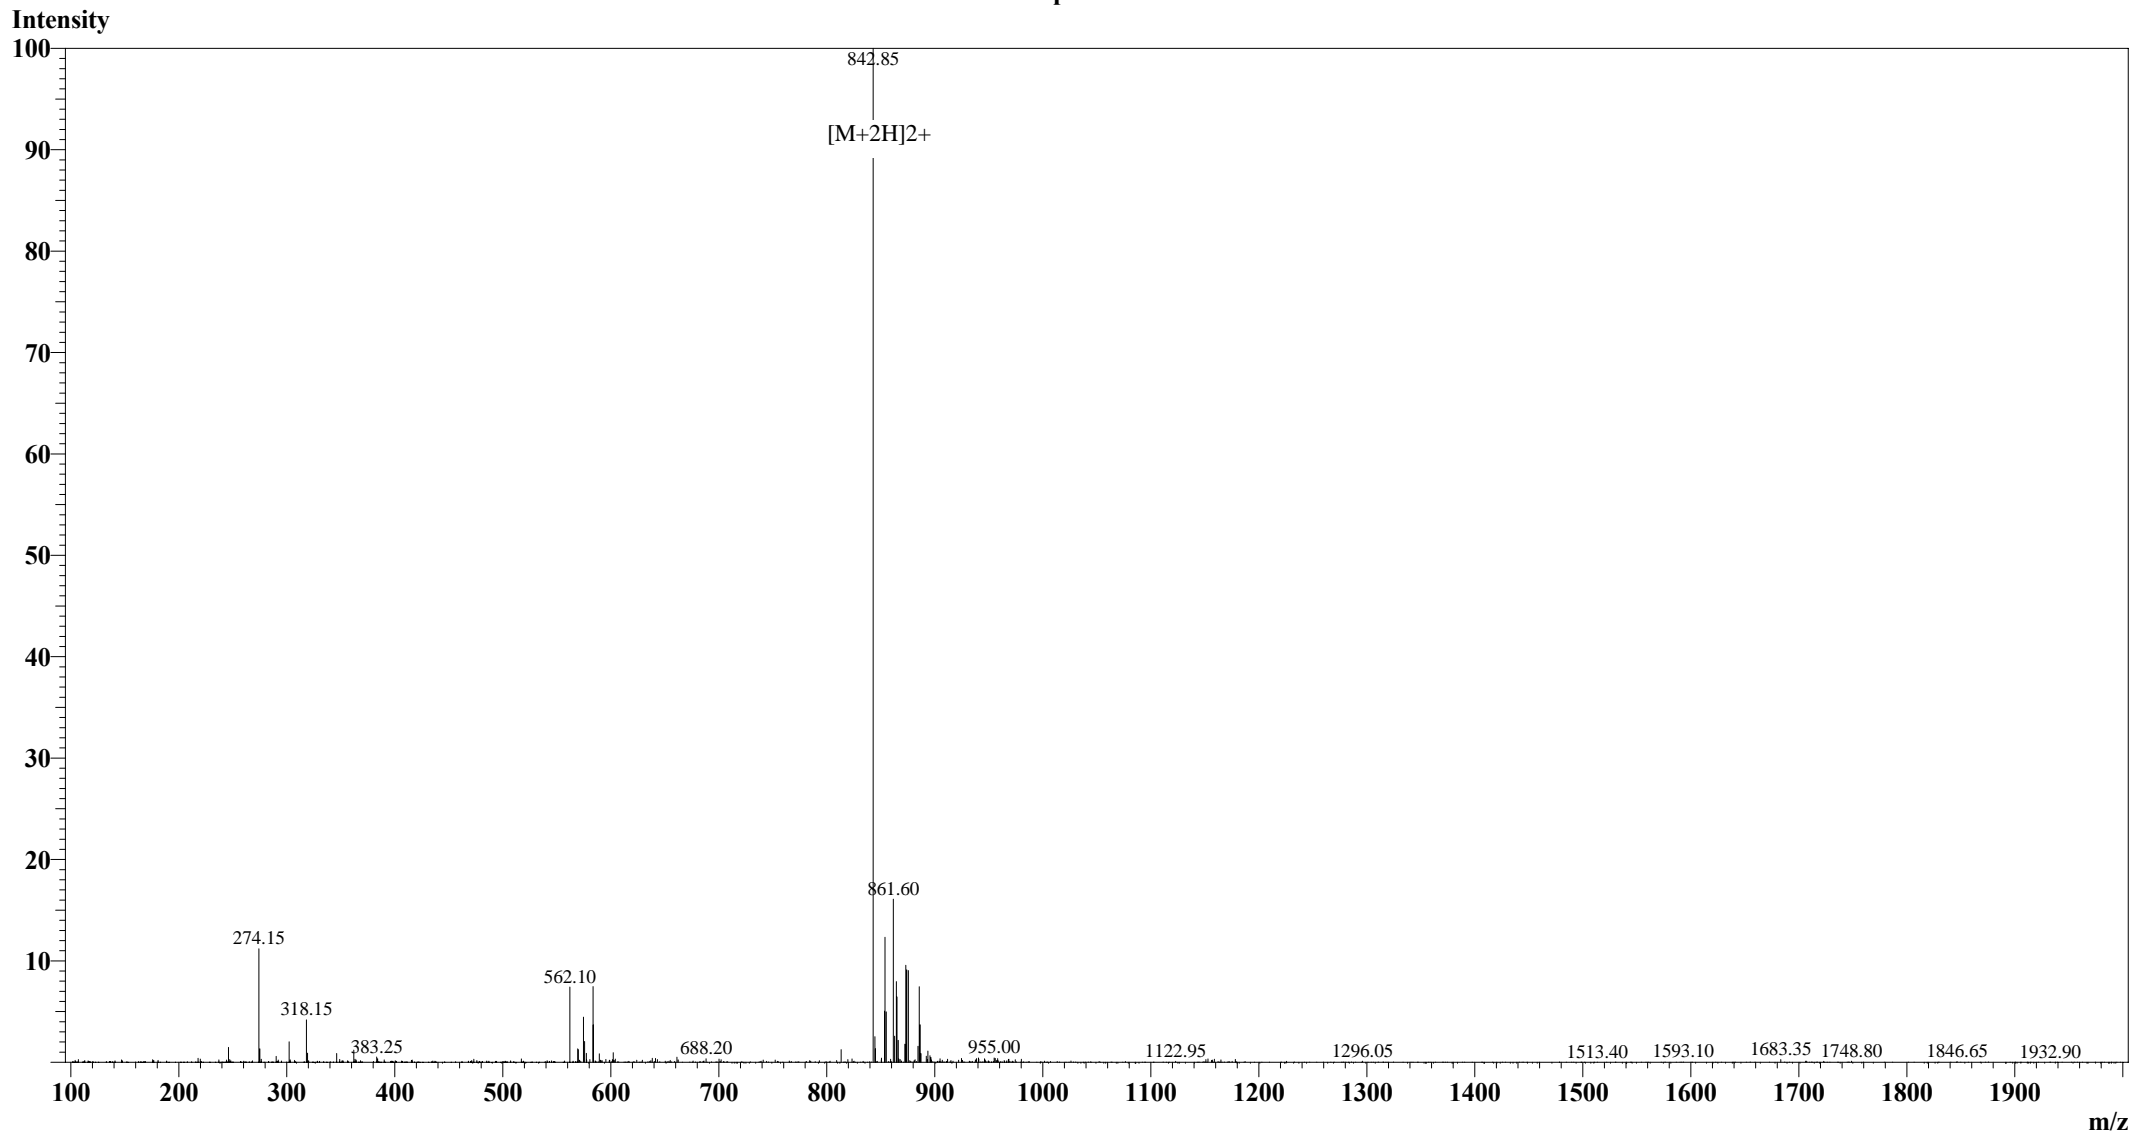

Sample Information

User : Grace
Date Acquired : 08/06/2009 12:16:38
Sample Name : pheromone moth
Cat No. : RP01002
Lot No. : CB01908
Injection Volum : 1.000µL
Theoretical MW : 1683.98
Observed MW : 1683.70

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH