


Positive

### MS Spectrum

Intensity

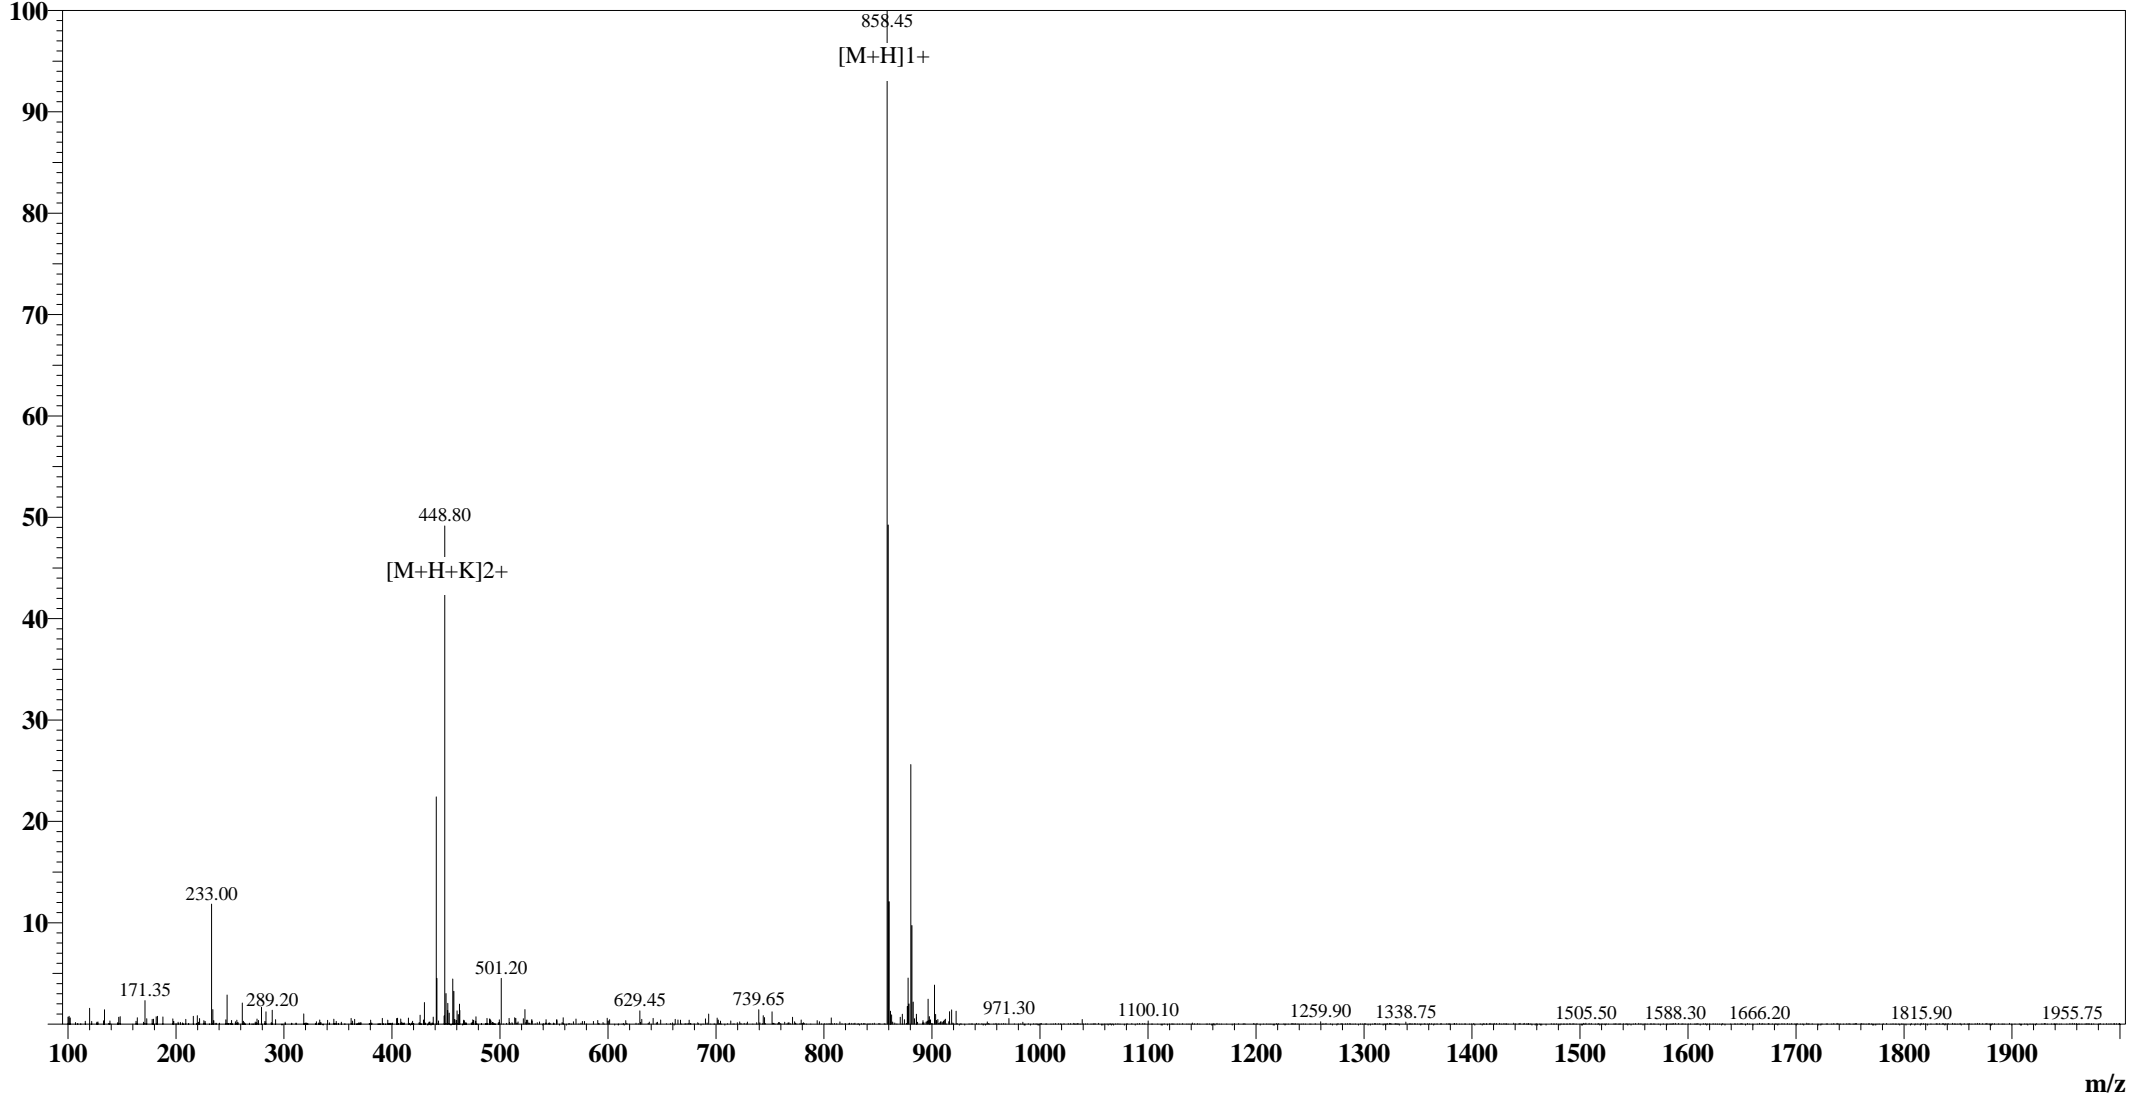

#### Sample Information

User :xu  
Date Acquired : 2008-4-24 10:56:37  
Sample Name :Peptide T  
Cat No. : RP13035  
Injection Volum : 1.000µL  
Theoretical MW :857.39  
Observed MW :857.45

Interface :ESI  
Nebulizing Gas Flow :1.50 L/min  
CDL Temp : 250°C  
CDL Volt : -25.0V  
Block Temp : 200°C

Prerod Bias :+4.5kv  
Detector :1.5kv  
T.Flow : 0.2ml/min  
B.conc : 50%H2O/50%MeOH