


MS Spectrum

Positive

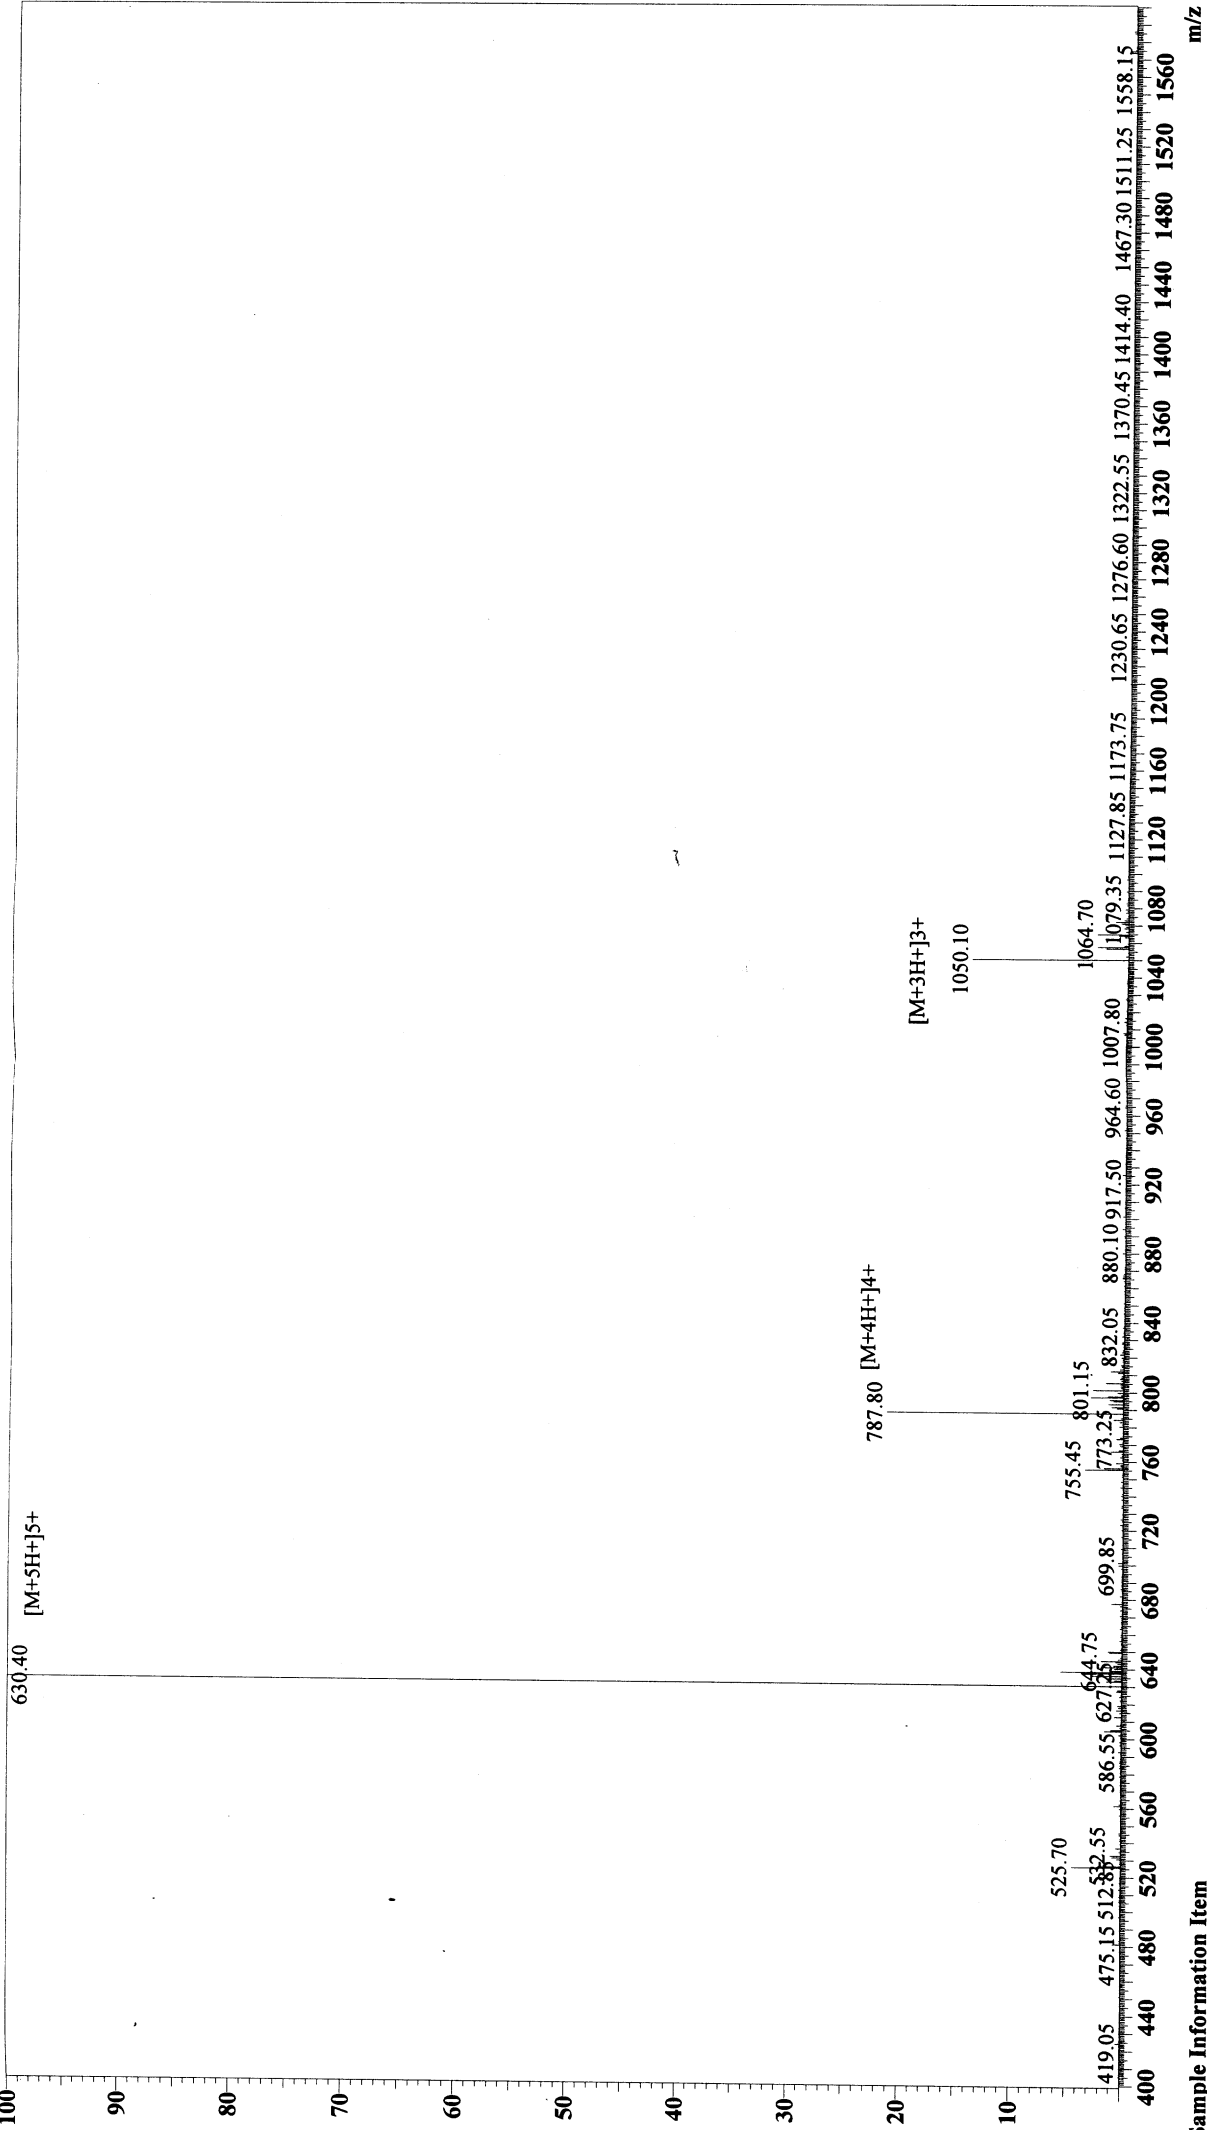

Sample Information Item

Date and Time : 2005-4-27 22:42:05
User : xie
Sample : DA-29-1
Inj. Volume : 1.000
MW : 3146.62

RP10341

PX00409508

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN