


MS Spectrum

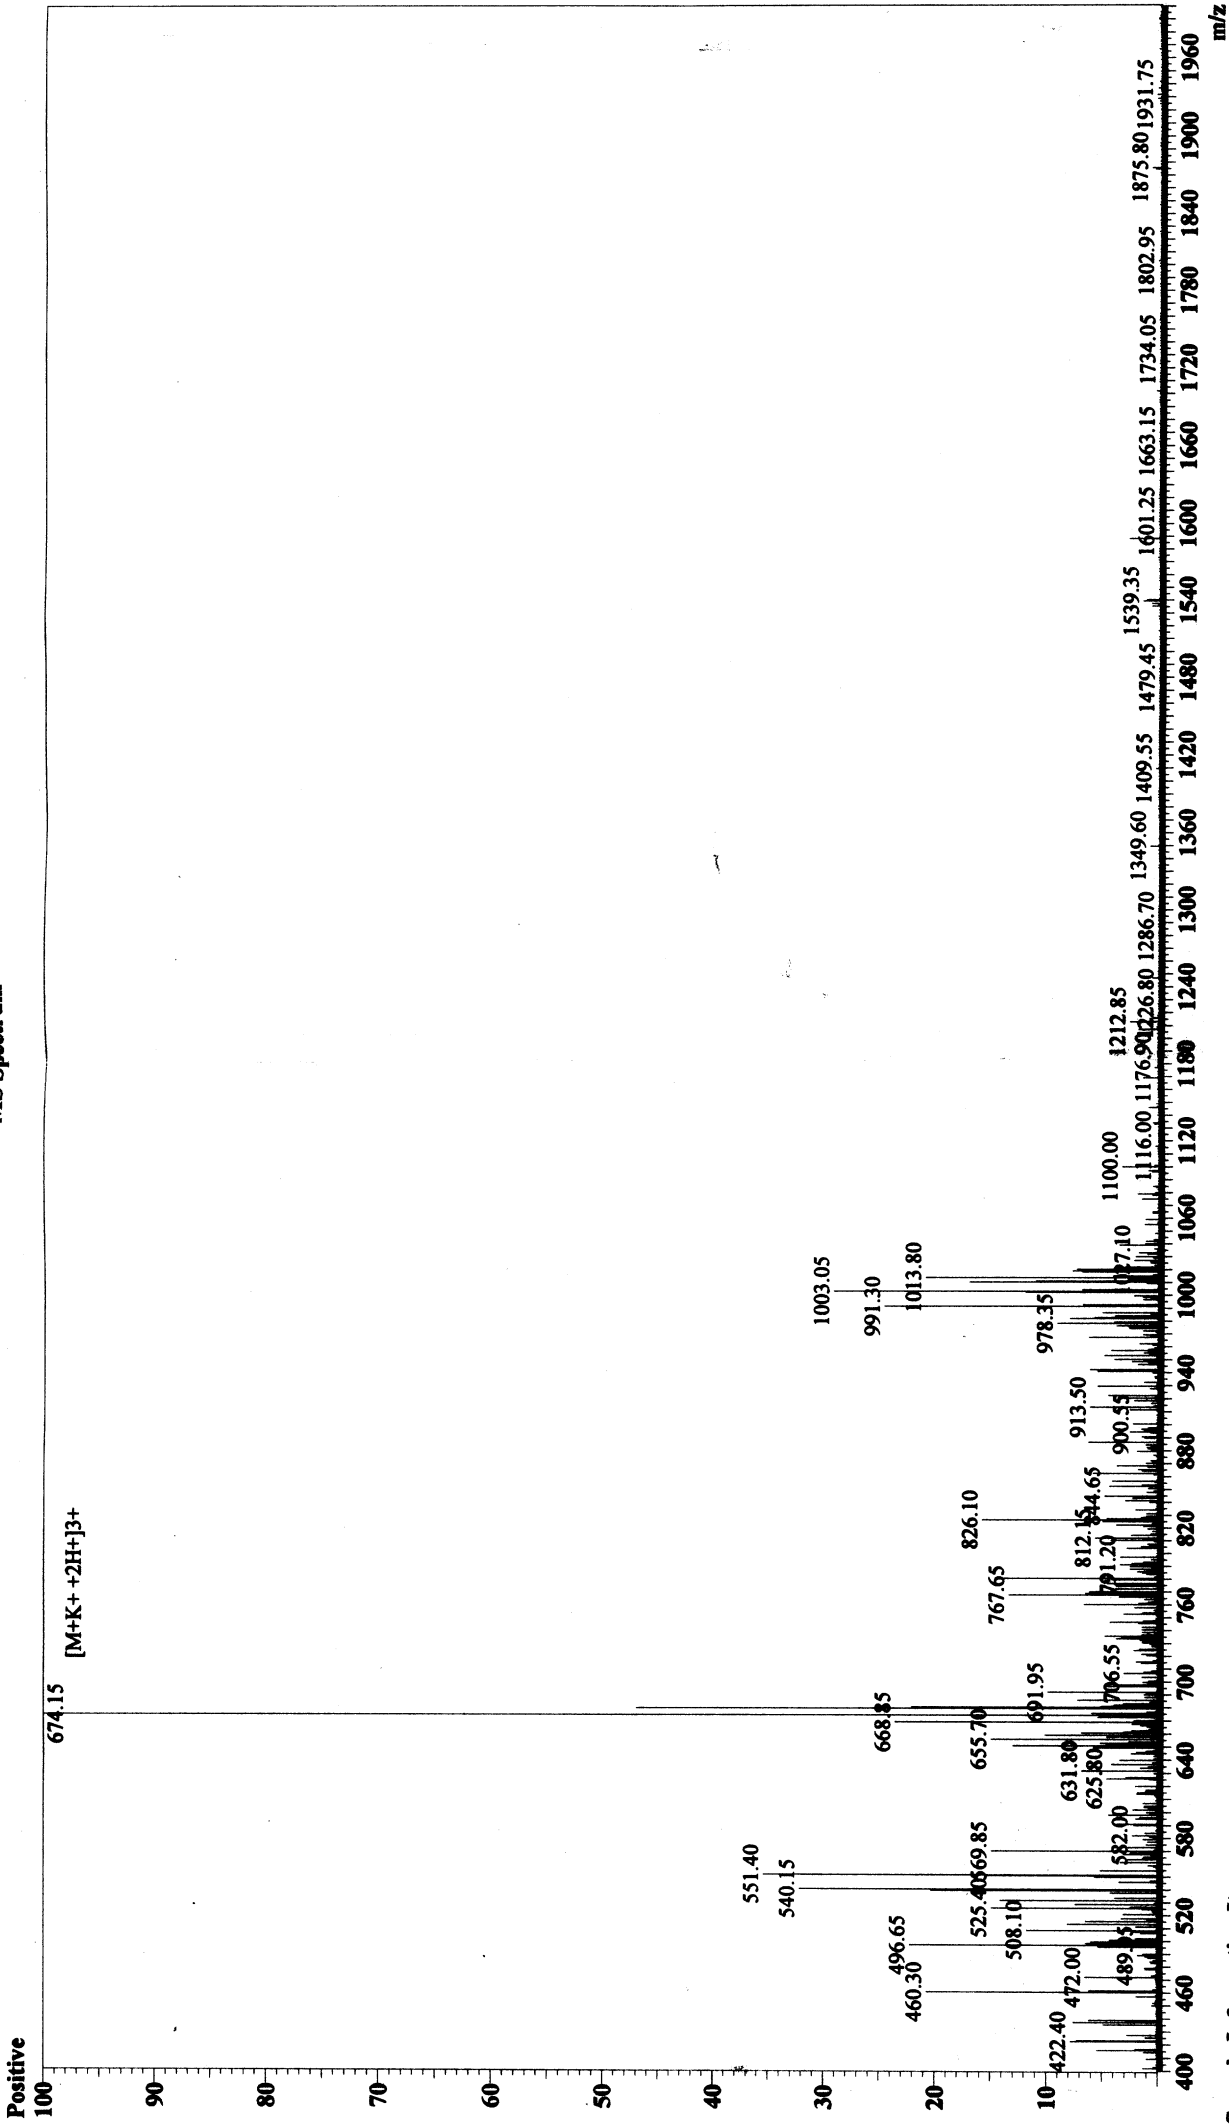

Sample Information Item  
 Date and Time : 2005-6-14 20:37:14  
 User : FJS  
 Sample : RP10809(GA-20-NH2)  
 Inj. Volume : 1.000  
 MW : 1981.34

Probe: ESI  
 Nebulizer Gas Flow: 1.5L/min  
 CDL: -20.0v  
 CDL Temp: 250C  
 Block Temp: 200C

Probe bias: +4.5kv  
 Detector: 1.5kv  
 T. Flow: 0.2ml/min  
 B. conc: 50%H2O/50%ACN

RP10809  
 PX00109508