


MS Spectrum

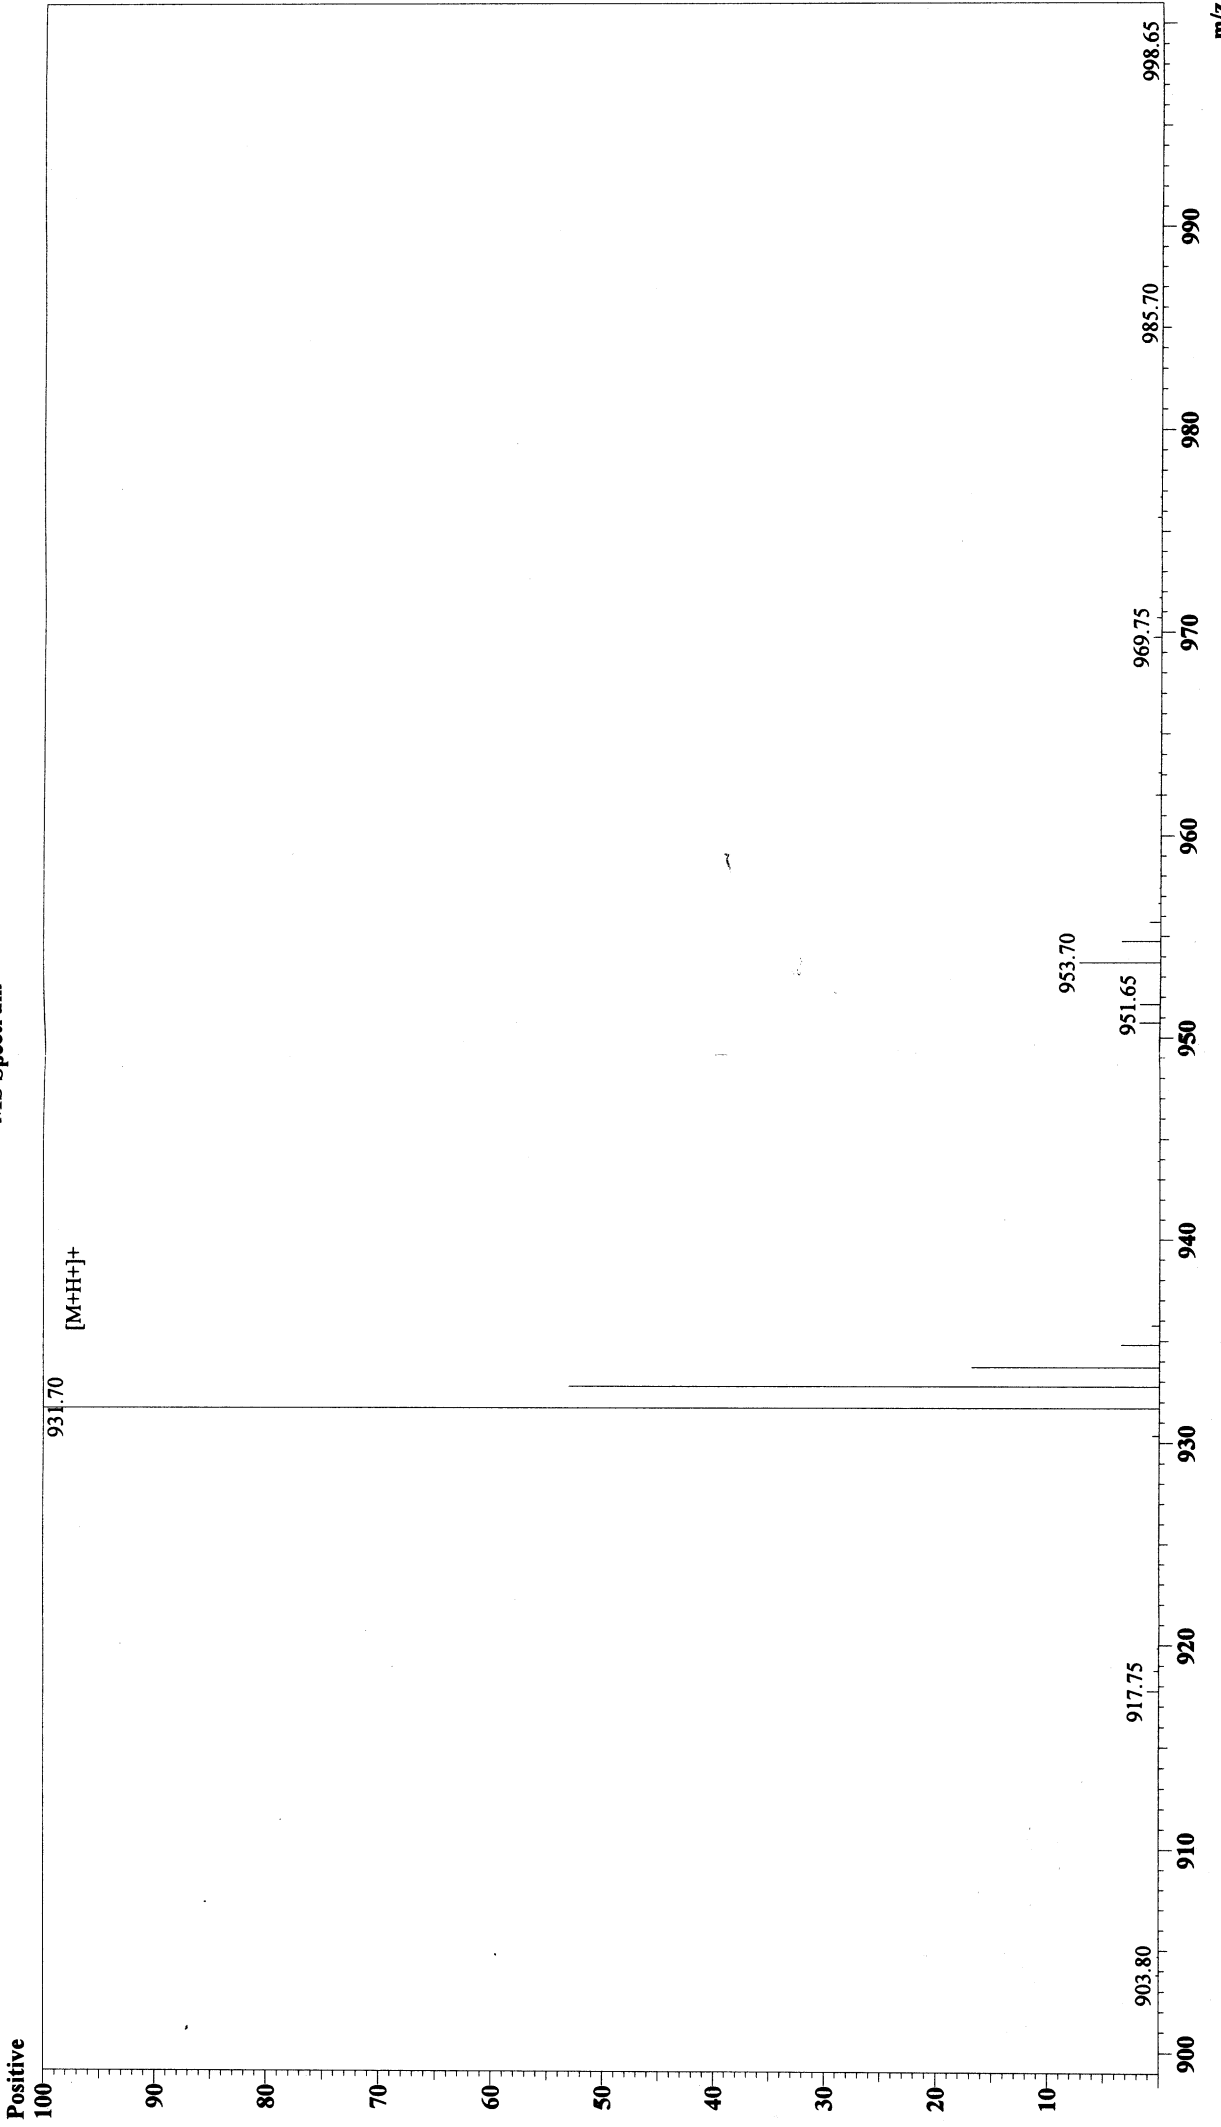

Sample Information Item  
Date and Time : 2005-4-20 19:18:08  
User : FJS  
Sample : RP11259(RF-7)  
Inj. Volume : 1.000  
MW : 931.11

RP11259  
PY00609508

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0V  
Block Temp: 250°C  
200°C