


Positive

MS Spectrum

Intensity

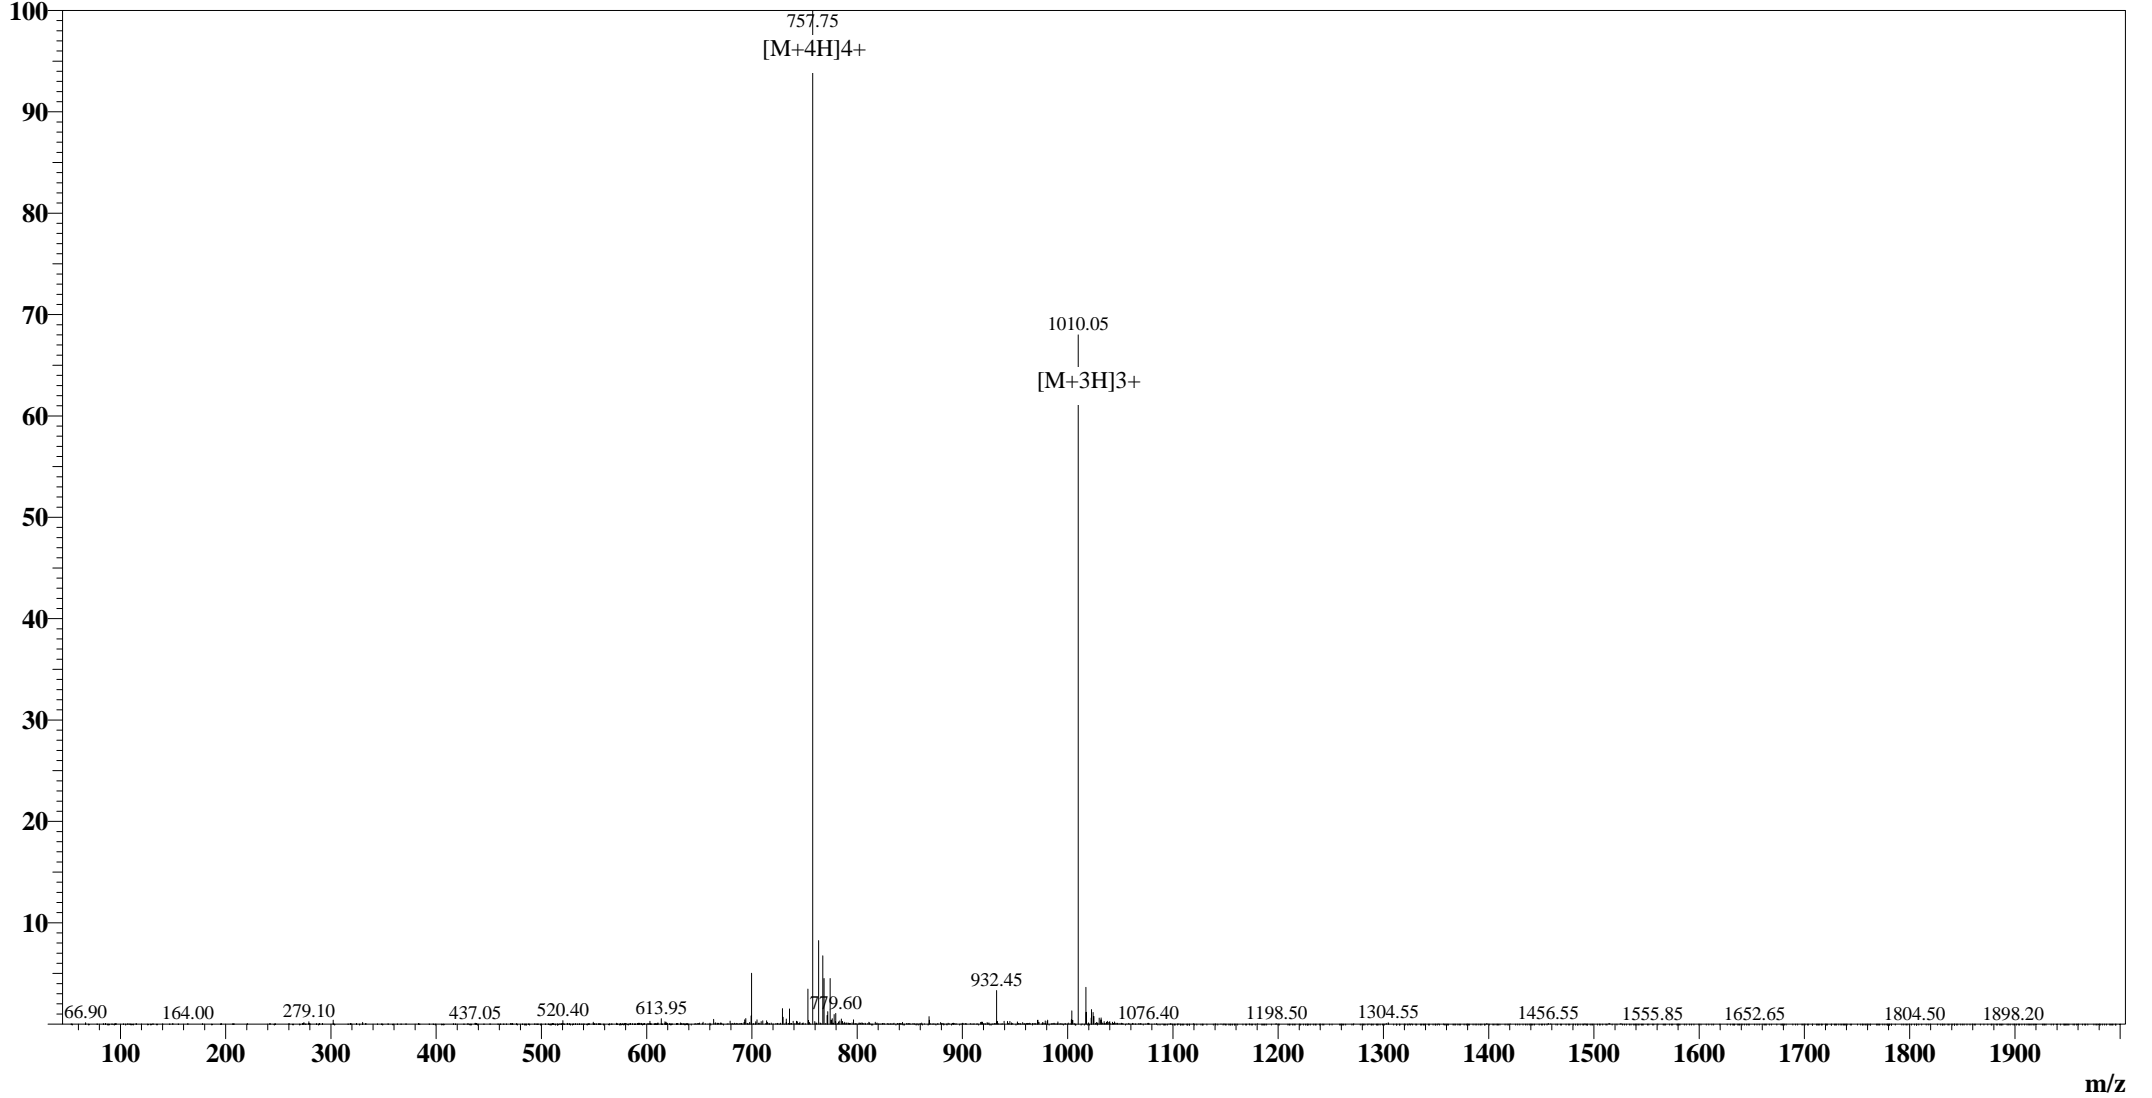

Sample Information

User : Grace
Date Acquired : 2008-12-12 14:58:35
Sample Name : Secretin, rat
Cat No. : RP10248
Injection Volum : 1.000µL
Theoretical MW : 3027.37
Observed MW : 3027.15

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250°C
CDL Volt : -25.0V
Block Temp : 200°C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H2O/50%MeOH