

Sample Name : Gastrin Releasing Peptide, porcine
 Cat. No. : RP10792
 Lot. No. : CD02906

Pump A : 0.065% trifluoroacetic in 100% water
 Pump B : 0.05% trifluoroacetic in 100% acetonitrile
 Total Flow : 1 ml / min
 Wavelength : 214 nm


Time	Unit	Command	Value	Comment
0.01	Pumps	Pump A B.Conc	5	
25.00	Pumps	Pump A B.Conc	65	
25.10	Pumps	Pump A B.Conc	95	
35.00	Pumps	Pump A B.Conc	95	
35.10	Pumps	Pump A B.Conc	5	
47.00	Pumps	Pump A B.Conc	5	
47.10	Controller	Stop		

<<Column Performance>>

<Detector A>

Column : Alltima™ C18 4.6 x 250 mm

Chromatogram

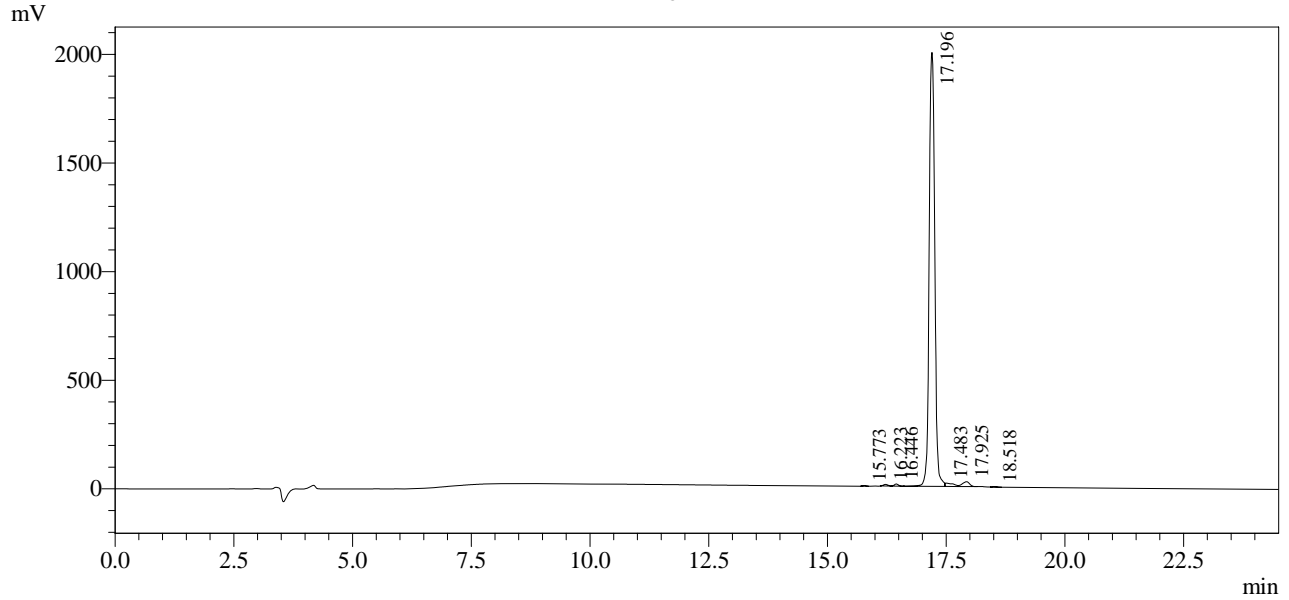

1 Det.A Ch1 / 214nm

Peak Table

Detector A Ch1 214nm

Peak#	Ret. Time	Area	Height	Area %
1	15.773	12984	2504	0.077
2	16.223	51568	7540	0.308
3	16.446	60407	10201	0.361
4	17.196	16201584	1997612	96.690
5	17.483	182214	15164	1.087
6	17.925	236410	22292	1.411
7	18.518	11031	1897	0.066
Total		16756197	2057209	100.000