


On November 12, 2021, the GenScript cPass™ Neutralization Antibody Detection Kit (cPass) received an updated emergency use authorization (EUA) from the Food and Drug Administration (FDA) for semi-quantitative use. The updated authorization also increased the assay's shelf-life from 6 to 9 months, and updated the manufacturing address to the new GenScript Diagnostics Facility.

These new box label changes are illustrated below.

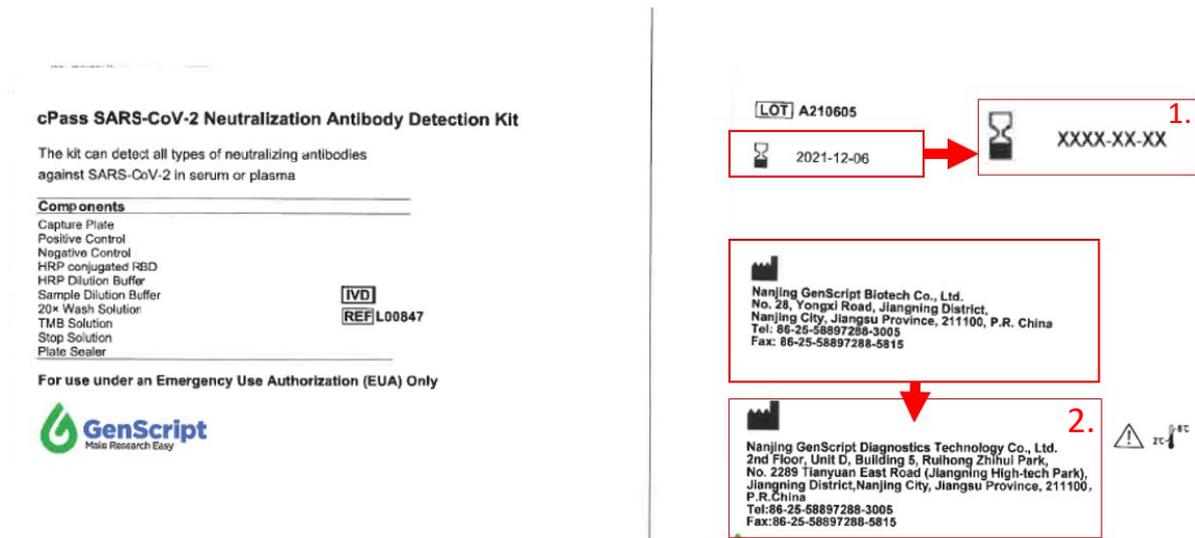

1. New expiration date representing 9 months.
2. New manufacturer address.

Example of complete kit labels for lots manufactured after February 1, 2022.



<p>Capture Plate</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>Capture Plate 1 plate</p> <p>REF S1-88 XXXX-XX-XX</p> <p>LOT A210706-C01</p> <p>⚠ 2-4°C</p>	<p>Positive Control</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>Positive Control 0.16 mL</p> <p>REF S1-10 XXXX-XX-XX</p> <p>LOT A220101-P01</p> <p>⚠ 2-4°C</p>	<p>Negative Control</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>Negative Control 0.08 mL</p> <p>REF S1-11 XXXX-XX-XX</p> <p>LOT A220101-N01</p> <p>⚠ 2-4°C</p>
<p>HRP conjugated RBD</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>HRP conjugated RBD 0.02 mL</p> <p>REF S1-30 XXXX-XX-XX</p> <p>LOT A220101-R01</p> <p>⚠ 2-4°C</p>	<p>HRP Dilution Buffer</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>HRP Dilution Buffer 10 mL</p> <p>REF S1-90 XXXX-XX-XX</p> <p>LOT A220101-D01</p> <p>⚠ 2-4°C</p>	<p>Sample Dilution Buffer</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>Sample Dilution Buffer 50 mL</p> <p>REF S1-60 XXXX-XX-XX</p> <p>LOT A220101-S01</p> <p>⚠ 2-4°C</p>
<p>20×Wash Solution</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>20× Wash Solution 40 mL</p> <p>REF S1-70 XXXX-XX-XX</p> <p>LOT A2201W01</p> <p>⚠ 2-4°C</p>	<p>TMB Solution</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>TMB Solution 12 mL</p> <p>REF S1-40 XXXX-XX-XX</p> <p>LOT A2201T01</p> <p>⚠ 2-4°C</p>	<p>Stop Solution</p> <p>SARS-CoV-2 Neutralization Antibody Detection Kit</p> <p>Stop Solution 6 mL</p> <p>REF S1-50 XXXX-XX-XX</p> <p>LOT A2201L01</p> <p>⚠ 2-4°C</p>