


Positive

MS Spectrum

Intensity

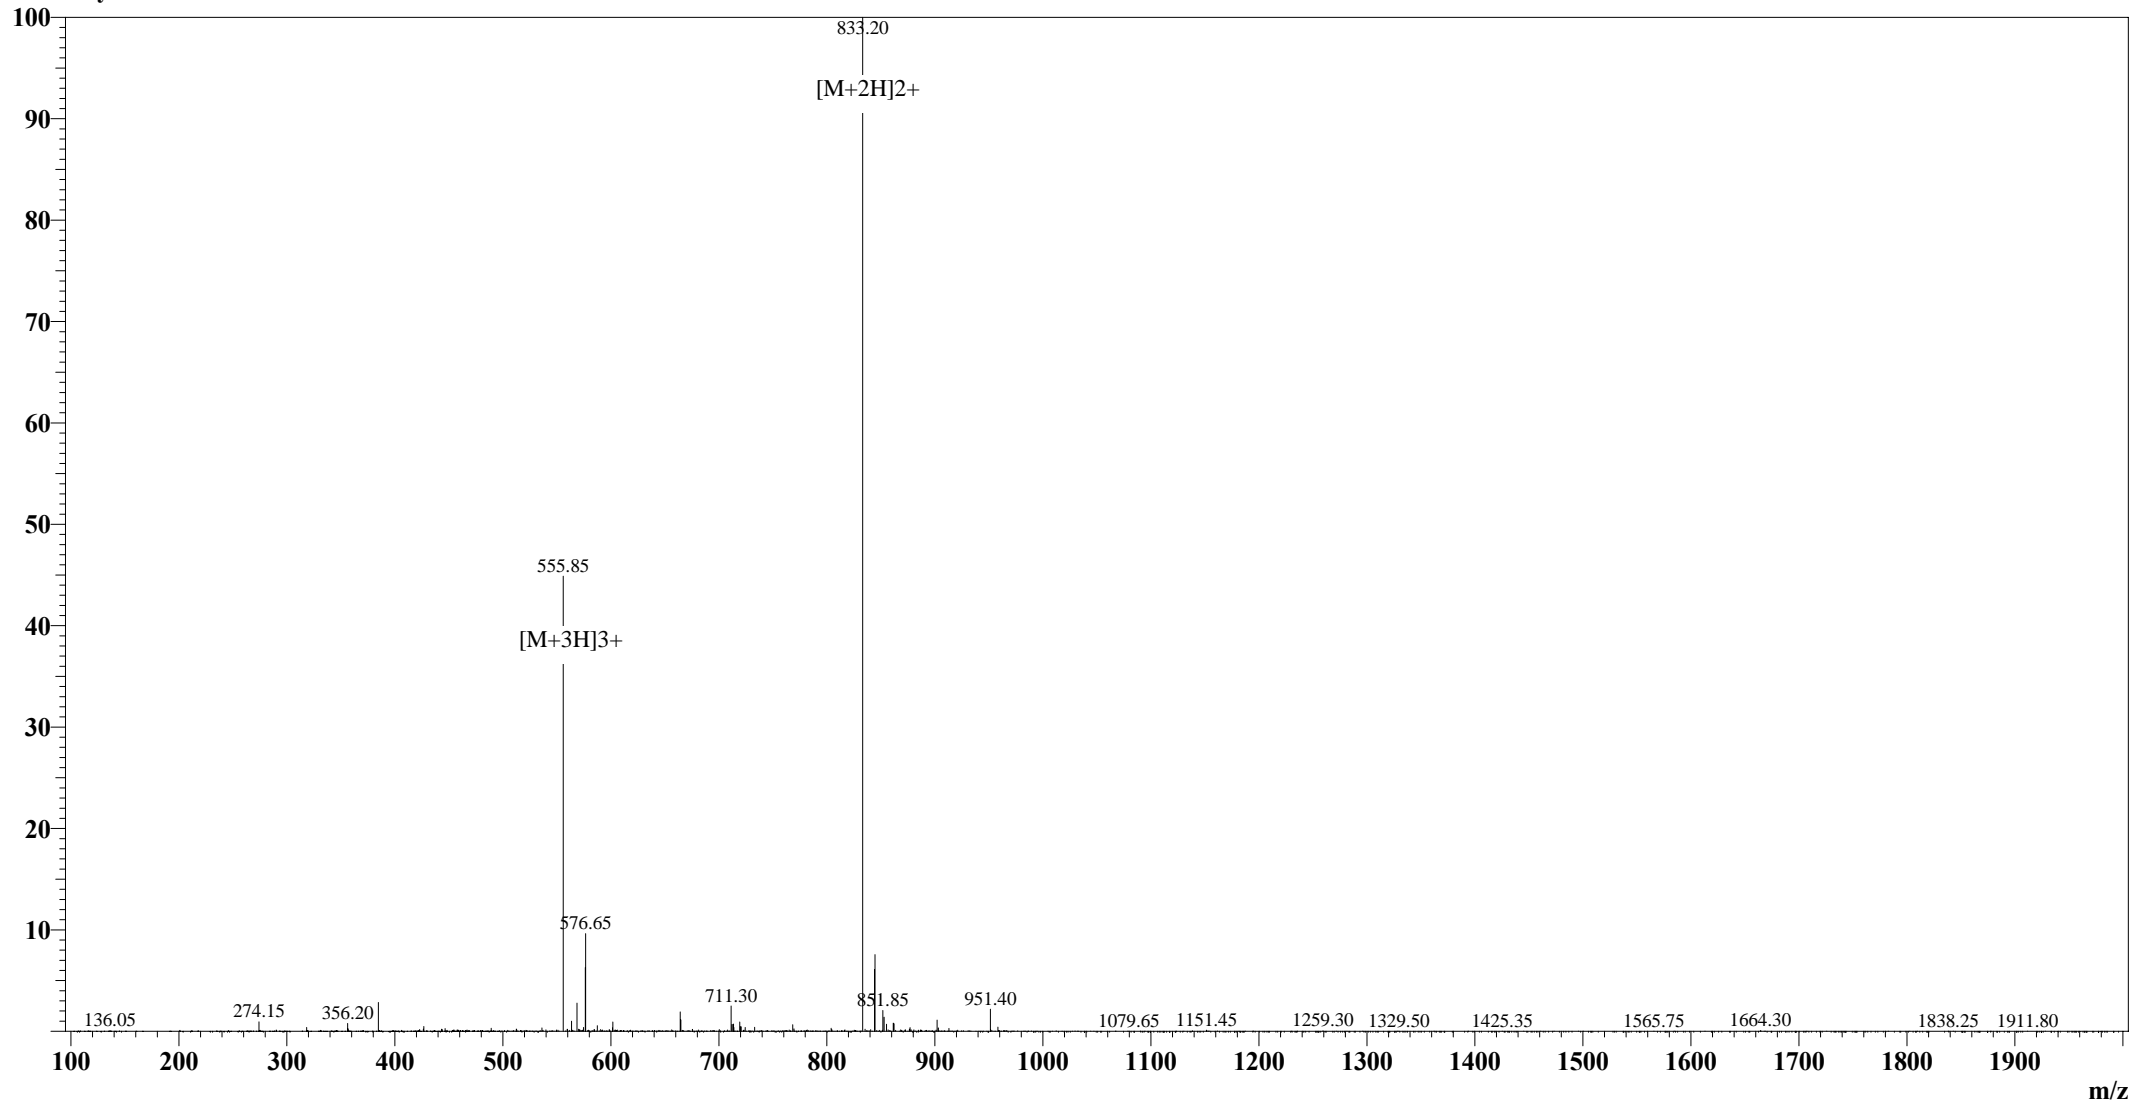

Sample Information

User : Grace
Date Acquired : 07/06/2009 15:47:11
Sample Name : α -MSH,amide
Cat No. : RP10644
Lot No. : CB04907
Injection Volum : 1.000 μ L
Theoretical MW : 1664.90
Observed MW : 1664.40

Interface : ESI
Nebulizing Gas Flow : 1.50 L/min
CDL Temp : 250 $^{\circ}$ C
CDL Volt : -25.0V
Block Temp : 200 $^{\circ}$ C

Prerod Bias : +4.5kv
Detector : 1.5kv
T.Flow : 0.2ml/min
B.conc : 50%H₂O/50%MeOH